

888 Titrande



Manual

8.888.8004EN / v8 / 2025-09-12



Metrohm AG
CH-9100 Herisau
Switzerland
Phone +41 71 353 85 85
Fax +41 71 353 89 01
info@metrohm.com
www.metrohm.com

888 Titrand

Manual

Technical Communication
Metrohm AG
CH-9100 Herisau
techcom@metrohm.com

This documentation is protected by copyright. All rights reserved.

This documentation has been prepared with great care. However, errors can never be entirely ruled out. Please send comments regarding possible errors to the address above.

Table of contents

1	Introduction	1
1.1	The Titrand system	1
1.2	Device description	2
1.3	Titration modes – Measuring modes – Dosing commands	3
1.4	About the documentation	4
1.4.1	Accessories	4
1.4.2	Symbols and conventions	5
2	Safety	7
2.1	Intended use	7
2.2	Responsibility of the operator	7
2.3	Personnel requirement	8
2.4	Safety instructions	8
2.4.1	Electrical safety	8
2.4.2	Tubing and capillary connections	9
2.4.3	Flammable solvents and chemicals	9
3	Overview of the instrument	10
4	Installation	12
4.1	Setting up the instrument	12
4.1.1	Packaging	12
4.1.2	Checks	12
4.1.3	Location	12
4.2	Connecting a controller	12
4.2.1	Operation	12
4.3	Connecting MSB devices	17
4.3.1	Connecting a dosing device	18
4.3.2	Connecting a stirrer or titration stand	19
4.3.3	Connecting a Remote Box	20
4.4	Connecting USB devices	21
4.4.1	General	21
4.4.2	Connecting a USB hub	22
4.4.3	Connecting a printer	22
4.4.4	Connecting a balance	23
4.4.5	Connecting a PC keyboard (only for operation with Touch Control)	24
4.4.6	Connecting a barcode reader	25

4.5	Connecting sensors	26
4.5.1	Connecting a pH, metal or ion-selective electrode	26
4.5.2	Connecting a reference electrode	27
4.5.3	Connecting a polarizable electrode	27
4.5.4	Connecting a temperature sensor or an electrode with integrated temperature sensor	28
4.5.5	Connecting the iConnect	28
4.5.6	Differential potentiometry	32
5	Working with the exchange unit	33
6	Operation and maintenance	35
6.1	General notes	35
6.1.1	Care	35
6.1.2	Maintenance by Metrohm Service	35
7	Troubleshooting	36
7.1	General	36
7.2	SET titration	37
7.2.1		37
8	Appendix	39
8.1	Remote interface	39
8.1.1	Pin assignment of the remote interface	39
9	Technical specifications	43
9.1	Measuring interface	43
9.1.1	Potentiometry	43
9.1.2	Temperature	43
9.1.3	Polarizer	44
9.2	Internal dosing device	45
9.3	Power connection	45
9.4	Ambient conditions	45
9.5	Reference conditions	46
9.6	Dimensions	46
9.7	Interfaces	46
	Index	48

Table of figures

Figure 1	The Titrand system	1
Figure 2	Front 888 Titrand	10
Figure 3	Rear 888 Titrand	11
Figure 4	Connecting the Touch Control	13
Figure 5	Connecting the computer	16
Figure 6	MSB connections	17
Figure 7	Connecting a dosing device	19
Figure 8	Connecting an MSB stirrer	20
Figure 9	Connecting the rod stirrer to the titration stand	20
Figure 10	Connecting the Remote Box	21
Figure 11	Connecting a printer	23
Figure 12	Connecting a pH, metal or ion-selective electrode	26
Figure 13	Connecting a reference electrode	27
Figure 14	Connecting a polarizable electrode	27
Figure 15	Connecting a temperature sensor or an electrode with integrated temperature sensor	28
Figure 16	Plugging in the mini USB adapter cable	29
Figure 17	Plugging in the 854 iConnect	29
Figure 18	Removing the protective cap	30
Figure 19	Aligning the guide pin	30
Figure 20	Attaching the electrode	30
Figure 21	Unplugging the 854 iConnect	31
Figure 22	Attaching the exchange unit	33
Figure 23	Connectors of the Remote Box	39
Figure 24	Pin assignment of remote socket and remote plug	39

1 Introduction

1.1 The Titrando system

The Titrando is the heart of the modular Titrando system. Operation is carried out either by a Touch Control with a touch-sensitive screen ("stand-alone titrator") or by a computer with a corresponding software.

A Titrando system can contain numerous, various kinds of devices. The following figure provides an overview of the peripheral devices you can connect to the 888 Titrando.

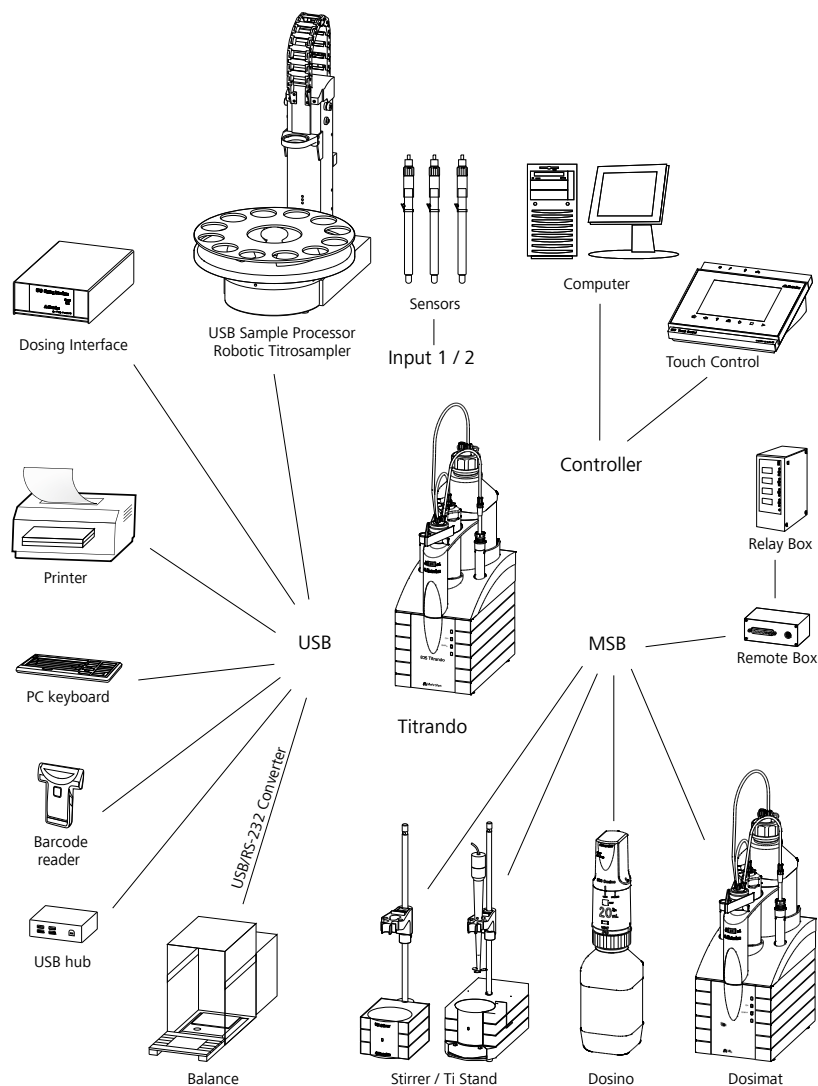


Figure 1 The Titrando system

Up to three control instruments (Titrandos, Dosing Interface, USB Sample Processor, etc.) can be controlled via USB connection during operation with the 900 Touch Control.

You can request information on special applications in the "Application Bulletins" and "Application Notes", available free of charge via the Metrohm representative responsible. Various monographs on the subjects of titration techniques and electrodes are also available.

Updating the device software is described in the help of the corresponding PC software.

1.2 Device description

The 888 Titrando has the following characteristics:

- **Operation**

Operation is carried out by means of a touch-sensitive Touch Control or with a high-performance PC software.

- **Dosing**

An internal dosing drive for exchange units.

- **MSB connectors**

Four MSB connectors (Metrohm Serial Bus) for connecting dosing devices (Dosimat with exchange unit or Dosino with dosing unit), stirrers, titration stands and Remote Boxes.

- **USB connectors**

Two USB connectors, through which devices such as printers, PC keyboards, barcode readers or additional control devices (USB Sample Processor, Titrando, Dosing Interface, etc.) can be connected.

- **Measuring interface**

One measuring input each for:

- a potentiometric electrode (pH, metal or ion-selective electrode)
- a separate reference electrode
- a temperature sensor (Pt1000 or NTC)
- a polarizable electrode
- an iConnect (measuring interface for electrodes with integrated data chip, so-called iTrodes)

1.3 Titration modes – Measuring modes – Dosing commands

The 888 Titrande supports the following titration modes, measuring modes and dosing commands:

- **DET**

Dynamic equivalence point titration. The reagent is added in variable volume steps.

Measuring modes:

- **pH** (pH measurement)
- **U** (potentiometric voltage measurement)
- **Ipol** (voltametric measurement with selectable polarization current)
- **Upol** (amperometric measurement with selectable polarization voltage)

- **MET**

Monotonic equivalence point titration. The reagent is added in constant volume steps.

Measuring modes:

- **pH** (pH measurement)
- **U** (potentiometric voltage measurement)
- **Ipol** (voltametric measurement with selectable polarization current)
- **Upol** (amperometric measurement with selectable polarization voltage)

- **SET**

Endpoint titration at one or two specified endpoints.

Measuring modes:

- **pH** (pH measurement)
- **U** (potentiometric voltage measurement)
- **Ipol** (voltametric measurement with selectable polarization current)
- **Upol** (amperometric measurement with selectable polarization voltage)

- **MEAS**

The following measuring modes can be selected for measurements:

- **pH** (pH measurement)
- **U** (potentiometric voltage measurement)
- **Ipol** (voltametric measurement with selectable polarization current)
- **Upol** (amperometric measurement with selectable polarization voltage)
- **T** (temperature measurement)



- **CAL**

Electrode calibration.

Measuring mode:

- **pH** (calibration of pH electrodes)

- **Dosing commands**

The following commands for dosing can be selected:

- **PREP** (rinsing the cylinder and tubings of an exchange unit or dosing unit)
- **EMPTY** (emptying the cylinder and tubings of a dosing unit)
- **ADD** (dosing a specified volume)

1.4 About the documentation



CAUTION

Please read through this documentation carefully before putting the device into operation. The documentation contains information and warnings which the user must follow in order to ensure safe operation of the device.

1.4.1 Accessories

Up-to-date information on the scope of delivery and optional accessories for your product can be found on the Internet. You can download this information using the article number as follows:

Downloading the accessories list

- 1 Enter <https://www.metrohm.com/> into your Internet browser.
- 2 Enter the article number (e.g. **888**) into the search field.
The search result is displayed.
- 3 Click on the product.
Detailed information regarding the product is shown on various tabs.
- 4 On the **Included parts** tab, click on **Download the PDF**.
The PDF file with the accessories data is created.



NOTE

Once you have received your new product, we recommend downloading the accessories list from the Internet, printing it out and keeping it together with the manual for reference purposes.

1.4.2 Symbols and conventions

The following symbols and formatting may appear in this documentation:

(5- 12)	Cross-reference to figure legend The first number refers to the figure number, the second to the device part in the figure.
1	Instruction step Perform the steps one after the other.
Method	Dialog text, parameter in the software
File ► New	Menu or menu item
[Continue]	Button or key
	WARNING This symbol draws attention to a possible life-threatening hazard or risk of injury.
	WARNING This symbol draws attention to a possible hazard due to electrical current.
	WARNING This symbol draws attention to a possible hazard due to heat or hot instrument parts.
	WARNING This symbol draws attention to a possible biological hazard.
	WARNING Warning of optical radiation
	CAUTION This symbol draws attention to possible damage to devices or device parts.



NOTICE

This symbol highlights additional information and tips.

2 Safety



WARNING

Operate this instrument only according to the information contained in this documentation.

This device left the factory in a flawless state in terms of technical safety. To maintain this state and ensure non-hazardous operation of the device, the following instructions must be observed carefully.

2.1 Intended use

2.2 Responsibility of the operator

The operator is responsible for the following tasks to ensure the safe operation of the product:

- Check the condition of the product before use:
- Ensure that the operating values and limit values specified in the technical specifications () are observed.
- Maintain and clean the product regularly:
- Remedy defects and malfunctions immediately:



NOTE

The product may be used only when its status is perfect.

- Train staff on basic occupational safety and accident prevention regulations for chemical laboratories and ensure that these regulations are complied with.
- Train personnel in the use of the product according to the user documentation (e.g., install, operate, eliminate faults).
- Provide personal protective equipment (e.g., protective glasses, gloves).
- Provide suitable tools and equipment to execute the work safely.

2.3 Personnel requirement

Only qualified personnel may operate the product. Qualified personnel are persons who meet the following requirements:

- Knowledge of basic regulations on occupational safety and accident prevention.
- Knowledge regarding the application of fire prevention measures for laboratories.
- In-depth knowledge of handling hazardous chemicals.
- Personnel have been instructed and are able to operate the product safely and independently recognize and avoid potential dangers.
- The user documentation has been read and understood. The personnel operate the product according to the instructions in the user documentation.

2.4 Safety instructions

2.4.1 Electrical safety

The electrical safety when working with the instrument is ensured as part of the international standard IEC 61010.



WARNING

Only personnel qualified by Metrohm are authorized to carry out service work on electronic components.



WARNING

Never open the housing of the instrument. The instrument could be damaged by this. There is also a risk of serious injury if live components are touched.

There are no parts inside the housing which can be serviced or replaced by the user.

Supply voltage



WARNING

An incorrect supply voltage can damage the instrument.

Only operate this instrument with a supply voltage specified for it (see rear panel of the instrument).

Protection against electrostatic charges



WARNING

Electronic components are sensitive to electrostatic charges and can be destroyed by discharges.

Do not fail to pull the power cord out of the power socket before you set up or disconnect electrical plug connections at the rear of the instrument.

2.4.2 Tubing and capillary connections



CAUTION

Leaks in tubing and capillary connections are a safety risk. Tighten all connections well by hand. Avoid applying excessive force to tubing connections. Damaged tubing ends lead to leakage. Appropriate tools can be used to loosen connections.

Check the connections regularly for leakage. If the instrument is used mainly in unattended operation, then weekly inspections are mandatory.

2.4.3 Flammable solvents and chemicals



WARNING

All relevant safety measures are to be observed when working with flammable solvents and chemicals.

- Set up the instrument in a well-ventilated location (e.g. fume cupboard).
- Keep all sources of flame far from the workplace.
- Clean up spilled liquids and solids immediately.
- Follow the safety instructions of the chemical manufacturer.

[illegible]

1 Guide openings For centering the exchange unit.	2 Piston rod Moves the piston of the exchange unit up and down.
3 Contact pins For the data chip.	4 Coupling For switching the flat stopcock.
5 "On" LED Lights up when the Titrando is ready for operation.	6 "Status" LED Shows the current status of the internal dosing drive.

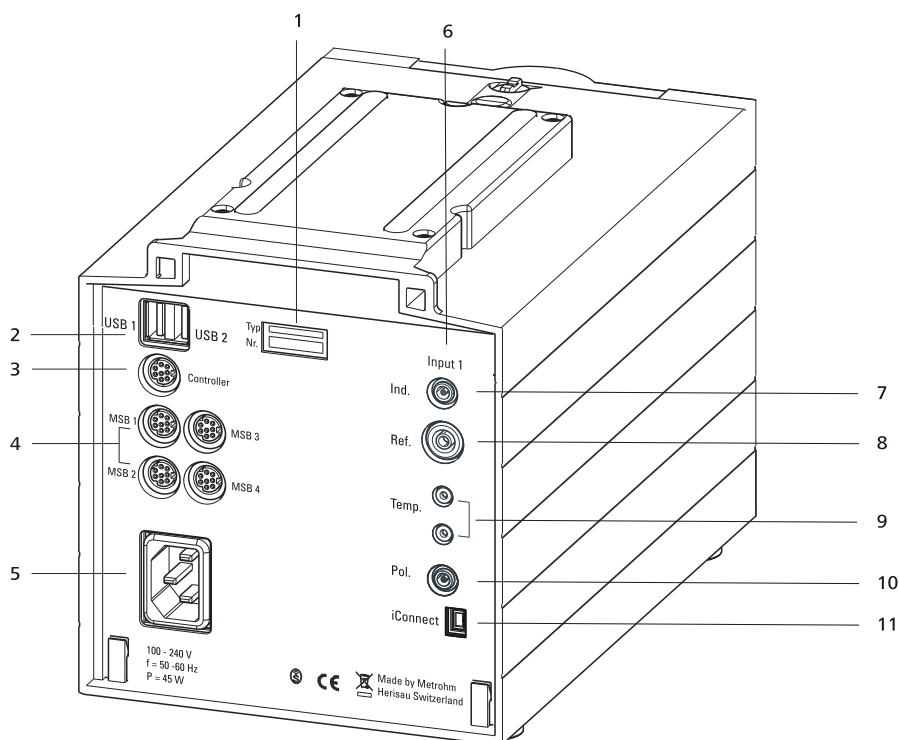


Figure 3 Rear 888 Titrand

1 Type plate

Contains specifications concerning supply voltage, instrument type and serial number.

3 Connector (Controller)

For connecting a Touch Control or a PC with installed PC software. Mini DIN, 9-pin.

5 Power socket**7 Electrode connector (Ind.)**

For connecting pH, metal or ion-selective electrodes with integrated or separated reference electrode. Socket F.

9 Temperature sensor connector (Temp.)

For connecting temperature sensors (Pt1000 or NTC). Two B sockets, 2 mm.

11 Electrode connector (iConnect)

For connecting electrodes with integrated data chip (iTrodes).

2 USB connector (USB 1 and USB 2)

USB ports (type A) for connecting printer, keyboard, barcode reader, additional Titrando, USB Sample Processor, etc.

4 MSB connector (MSB 1 to MSB 4)

Metrohm Serial Bus. For connecting external dosing devices, stirrers or Remote Boxes. Mini DIN, 9-pin.

6 Measuring interface 1 (Input 1)**8 Electrode connector (Ref.)**

For connecting reference electrodes, e.g. Ag/AgCl reference electrode. Socket B, 4 mm.

10 Electrode connector (Pol.)

For connecting polarizable electrodes, e.g. double Pt wire electrodes. Socket F.

4.2.1.1 Connecting a Touch Control



The plug is protected against accidental disconnection of the cable by means of a pull-out protection feature. If you wish to pull out the plug, you first need to pull back the outer plug sleeve marked with arrows.

Connect the Touch Control as follows:

- 1 ■ Insert the plug of the Touch Control connection cable into the **Controller** socket.

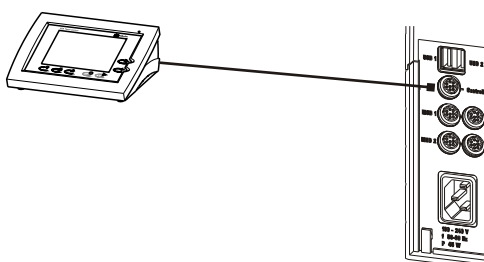


Figure 4 Connecting the Touch Control

- 2
 - Connect the MSB devices (see chapter 4.3, page 17).
 - Connect the USB devices (see chapter 4.4, page 21).

- 3** ■ Connect the Titrando to the power grid.

- 4** ■ Switch on the Touch Control.

The Touch Control power supply is supplied through the Titrand. Automatic system tests are performed on both instruments at the time of activation. The **On** LED on the front of the Titrand lights up when the system test has been completed and the instrument is ready for operation.



CAUTION

The Touch Control must be shut down properly by deactivation with the power switch on the rear of the instrument before the power supply is interrupted. If this is not done, then there is a danger of data loss. Because of the fact that the power supply for the Touch Control is provided through the Titrand, you must never disconnect the Titrand from the power grid (e.g. by deactivating with a connector strip) before you have deactivated the Touch Control.

If you would prefer not to position the Touch Control directly next to the Titrando, then you can lengthen the connection with the 6.2151.010 cable. The maximum connection length permitted is 5 m.

4.2.1.2 Connecting the instrument to the power grid



WARNING

Electric shock from electrical potential

Risk of injury by touching live components or through moisture on live parts.

- Never open the housing of the instrument while the power cord is still connected.
- Protect live parts (e.g. power supply unit, power cord, connection sockets) against moisture.
- Unplug the power plug immediately if you suspect that moisture has gotten inside the instrument.
- Only personnel who have been issued Metrohm qualifications may perform service and repair work on electrical and electronic parts.

Connecting the power cord

Accessories

Power cord with the following specifications:

- Length: max. 2 m
- Number of cores: 3, with protective conductor
- Instrument plug: IEC 60320 type C13
- Conductor cross-section 3x min. 0.75 mm² / 18 AWG
- Power plug:
 - according to customer requirement (6.2122.XX0)
 - min. 10 A



1 Plugging in the power cord

- ### 4.2.1.3 Connecting a computer

You need administrator rights for the installation of driver software and control software on your computer.

A driver installation is required in order to ensure that the 888 Titrande is recognized by the computer software. To accomplish this, you must comply with the procedures specified. The following steps are necessary:

- Insert the computer software installation CD and carry out the installation program directions.
- Exit the program if you have started it after the installation.

- Connect the instrument to the power grid if you have not already done this (*see chapter 4.2.1.2, page 14*).
The "On" LED on the 888 Titrand is not yet illuminated!
- Connect the instrument to a USB connector (type A) of your computer (see manual of your computer). The 6.2151.000 cable is used for this purpose.

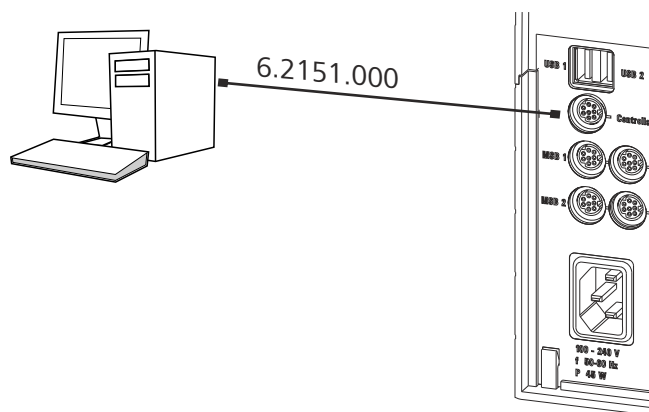


Figure 5 Connecting the computer

The instrument is recognized. Depending on the version of the Windows operating system used, the driver installation proceeds differently afterwards. Either the necessary driver software is installed automatically or an installation wizard is started.

- 3 Follow the instructions of the installation wizard.


The "On" LED on the 888 Titrande lights up when the driver installation has been completed and the instrument is ready for operation.

If problems should occur during installation, contact your company's IT support team.



NOTE

The plug on the instrument end of the 6.2151.000 controller cable is protected against accidental disconnection by means of a pull-out protection feature. If you wish to pull out the plug, you first need to pull back the outer plug sleeve marked with arrows.

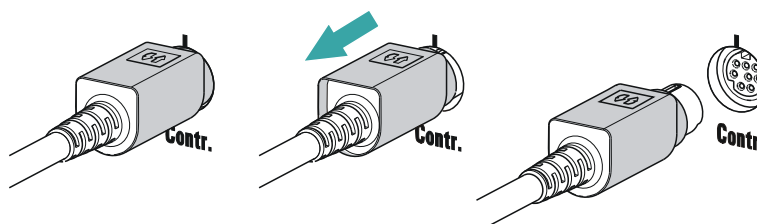

Registering and configuring the instrument in the computer software

The instrument must be registered in the configuration of your computer software. Once that has been done, you can then configure it according to your requirements. Proceed as follows:

1 Setting up the instrument

- Start the computer software.
The instrument is automatically recognized. The configuration dialog for the instrument is displayed.
- Make configuration settings for the instrument and its connectors.

More detailed information concerning the configuration of the instrument can be found in the documentation for the respective computer software.

4.3 Connecting MSB devices

In order to connect MSB devices, e.g. stirrers or dosing devices, Metrohm instruments are equipped with up to a maximum of four connectors on what is referred to as the *Metrohm Serial Bus* (MSB). Various kinds of peripheral devices can be connected in sequence (in series, as a "Daisy Chain") at a single MSB connector (8-pin Mini DIN socket) and controlled simultaneously by the respective control instrument. In addition to the connection cable, stirrers and the Remote Box are each equipped with their own MSB socket for this purpose.

The following figure provides an overview of the instruments that can be connected to an MSB socket, along with a number of different cabling variations.

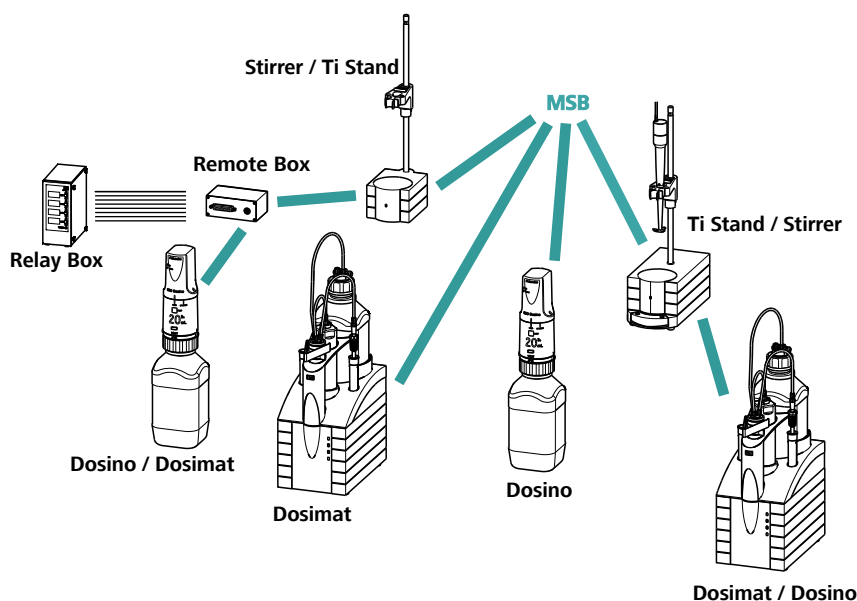


Figure 6 MSB connections

The control instrument determines which peripheral devices are supported.



NOTE

When connecting MSB devices together, the following must be observed:

- Only one device of the same type can be used at a single MSB connector at one time.
- Dosing devices of the 700 Dosino and 685 Dosimat plus type cannot be connected together with other MSB devices on a shared connector. These dosing devices must be connected separately.



CAUTION

Exit the control software before you plug in MSB devices. When it is switched on, the control instrument automatically recognizes which device is connected to which MSB connector. The operating unit or the control software enters the connected MSB devices into the system configuration (device manager).

MSB connections can be extended with the 6.2151.010 cable. The maximum connection length permitted is 15 m.

4.3.1 Connecting a dosing device

Three dosing devices can be connected to the instrument (**MSB 2 to MSB 4**).



NOTE

The dosing devices connected via MSB can be used only for simple volume additions, not for titrations.

The types of dosing devices that are supported are:

- 800 Dosino
- 700 Dosino
- 805 Dosimat
- 685 Dosimat plus

Proceed as follows:

1 Connecting a dosing device

- Exit the control software.
- Connect the connection cable of the dosing device to one of the sockets marked with **MSB** on the rear of the control device.

-

4.3.2 Connecting a stirrer or titration stand

These devices have a built-in magnetic stirrer (stirring "from below"):

- 801 Stirrer
- 803 Ti Stand

- 804 Ti Stand with rod stirrer 802 Stirrer

1 Connecting the stirrer or titration stand

- 19

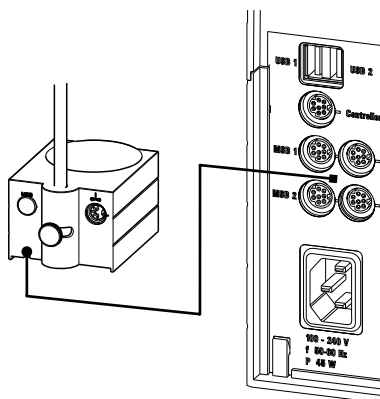


Figure 8 Connecting an MSB stirrer

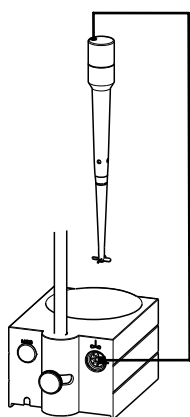


Figure 9 Connecting the rod stirrer to the titration stand

4.3.3 Connecting a Remote Box

Instruments that are controlled via remote lines and/or that send control signals via remote lines can be connected via the 6.2148.010 Remote Box. In addition to Metrohm, other instrument manufacturers also use similar connectors that make it possible to connect different instruments together. These interfaces are also frequently given the designations "TTL Logic", "I/O Control" or "Relay Control" and they generally have a signal level of 5 volts.

Control signals are understood to be electrical line statuses or electrical pulses (> 200 ms) which display the operating status of an instrument or which trigger or report an event. Sequences on a variety of instruments can thus be coordinated in a single complex automation system. However, no exchange of data is possible.

Proceed as follows:

1 Connecting the Remote Box

- Exit the control software.

-

You can connect the following instruments to the remote connector, among others:

- The Remote Box also has an MSB socket at which a further MSB device, e.g. a dosing device or a stirrer, can be connected.

4.4 Connecting USB devices

The 888 Titrando has two USB connectors (type A sockets) for peripheral devices with USB interfaces. The Titrando functions as a USB hub (distributor) no matter how it is operated. If you wish to connect more than two devices to the USB, you can also use an additional, commercially available USB hub.



CAUTION

If you operate the 888 Titrande with the aid of the Touch Control, take care to ensure that the Touch Control is switched off when you set up or disconnect connections between the various instruments. If you use a PC software to control the 888 Titrande, you should exit the program before you set up or disconnect the USB connections.

4.4.2 Connecting a USB hub

If you wish to connect more than two devices to the USB connector of the 888 Titrandu, you can also use an additional commercially available USB hub (distributor). If you operate the 888 Titrandu with the help of the Touch Control, then you should use a USB hub with its own power supply.

Connect the USB hub as follows:

- 1 Switch off the Touch Control and/or exit the PC software.
- 2 With the aid of the 6.2151.020 cable, connect the USB connector of the 888 Titrande (type A) with the USB connector of the hub (type B, see manual for the hub).
- 3 Switch on the Touch Control.

The USB hub is recognized automatically.

4.4.3 Connecting a printer

Printers that are connected to the 888 Titrando with Touch Control must meet the following requirements:

- Printer languages: HP-PCL (PCL 3 to 5, PCL 3GUI), Canon BJL Commands or Epson ESC P/2
- Printer resolution: 300 dots/inch or 360 dots/inch (Epson)
- Paper size: A4 or Letter, single-sheet feed.

Connect the printer as follows:

- 1 Switch off the Touch Control.
- 2 With the aid of the 6.2151.020 cable, connect the USB connector of the 888 Titrande (type A) with the USB connector of the printer (type B, see manual for the printer).
- 3 Switch on the printer first, then the Touch Control.

- 4

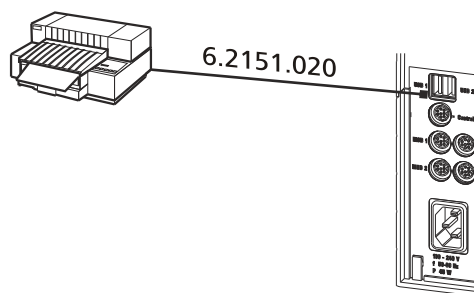


Figure 11 Connecting a printer

4.4.4 Connecting a balance

- Operation with a PC software:
 - Connect the balance directly to the serial connector (COM) of the computer. This is usually 9-pin and marked with the symbol **IOIOI**.
- Operation with Touch Control:
 - You will need the 6.2148.050 USB/RS-232 adapter to connect a balance.

The following table offers an overview of the balances that you can use together with the 888 Titrando and of which cable you will need for connection to the RS-232 interface:

Balance	Cable
AND ER, FR, FX with RS-232 interface (OP-03)	6.2125.020 + 6.2125.010
Mettler AB, AG, PR (LC-RS9)	In the scope of delivery for the balance
Mettler AM, PM, PE with interface option 016 or Mettler AJ, PJ with interface option 018	6.2146.020 + 6.2125.010 Also from Mettler: ME 47473 adapter and either ME 42500 hand switch or ME 46278 foot switch
Mettler AT	6.2146.020 + 6.2125.010 Also from Mettler: ME 42500 hand switch or ME 46278 foot switch
Mettler AX, MX, UMX, PG, AB-S, PB-S, XP, XS	6.2134.120

Balance	Cable
Mettler AE with interface option 011 or 012	6.2125.020 + 6.2125.010 Also from Mettler: ME 42500 hand switch or ME 46278 foot switch
Ohaus Voyager, Explorer, Analytical Plus	Cable AS017-09 from Ohaus
Precisa balances with RS-232-C interface	6.2125.080 + 6.2125.010
Sartorius MP8, MC, LA, Genius, Cubis	6.2134.060
Shimadzu BX, BW	6.2125.080 + 6.2125.010

Operation with Touch Control

Connect the balance as follows:

- 1 Plug in the USB plug of the USB/RS-232 adapter at the USB connector of the 888 Titrande.
- 2 Connect the RS-232 interface of the USB/RS-232 adapter with the RS-232 interface of the balance (see table for cable).
- 3 Switch on the Touch Control.
- 4 Switch on the balance.
- 5 Activate the RS-232 interface of the balance if necessary.
- 6 Configure the RS-232 interface of the USB/RS-232 adapter in the device manager of the Touch Control (see Touch Control manual).

4.4.5 Connecting a PC keyboard (only for operation with Touch Control)

The PC keyboard is used as an aid for text and numerical input.

Connect the PC keyboard as follows:

- 1 Insert the USB plug of the keyboard into one of the USB sockets of the 888 Titrando.

- The keyboard is recognized automatically and entered in the device manager.

4.4.6 Connecting a barcode reader

The barcode reader is used as an aid for text and numerical input. You can connect a barcode reader with USB interface.

Operation with Touch Control

Connect the barcode reader as follows:

- The barcode reader is recognized automatically and entered in the device manager.

Settings on the barcode reader:

Program the barcode reader as follows (see also the manual for the barcode reader):

- This setting must match the setting in the device manager (see the Touch Control manual).



4.5.2 Connecting a reference electrode

Connect the reference electrode as follows:

- 1** Plug the electrode plug into the **Ref.** socket of the 888 Titrand.

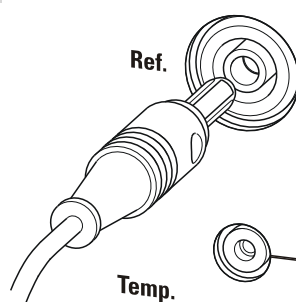


Figure 13 Connecting a reference electrode

4.5.3 Connecting a polarizable electrode

Connect the polarizable electrode as follows:

- 1** Plug the electrode plug into the **Pol.** socket of the 888 Titrand.

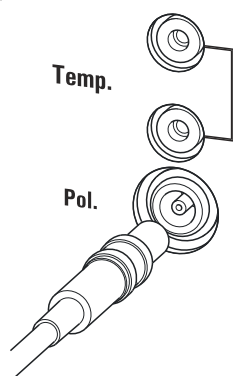


Figure 14 Connecting a polarizable electrode



NOTE

The electrode cable is protected against accidental disconnection of the cable by means of a pull-out protection. If you wish to pull out the plug again, you first need to pull back the outer plug sleeve.

4.5.4 Connecting a temperature sensor or an electrode with integrated temperature sensor

A temperature sensor of the Pt1000 or NTC type can be connected to the **Temp.** connector.

Connect the temperature sensor or the electrode with integrated temperature sensor as follows:

- 1** Insert the plugs of the temperature sensor into the **Temp.** sockets of the Titrando.

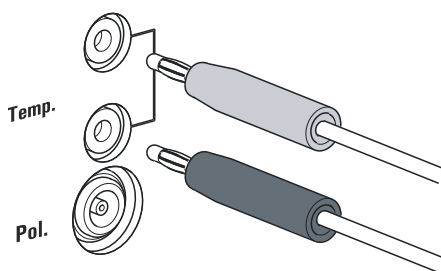


Figure 15 Connecting a temperature sensor or an electrode with integrated temperature sensor



NOTE

Always insert the red plug into the red socket. This is the only way that shielding against electrical interference can be ensured.

4.5.5 Connecting the iConnect

The external measuring interface 854 iConnect can be connected to the **iConnect** connector.

Connecting the 6.2168.000 mini USB adapter cable to an instrument

If the mini USB adapter cable is not connected to the instrument yet, proceed as follows:

- 1 Plug the mini USB adapter cable (2) into the **iConnect** connector of the instrument (1). Observe the correct orientation (markings).

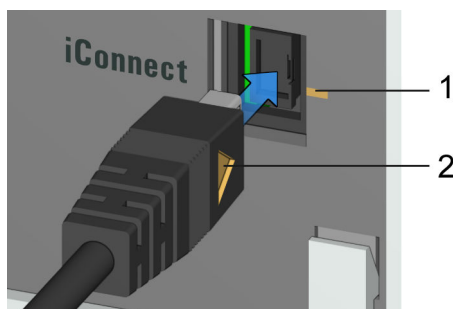


Figure 16 Plugging in the mini USB adapter cable

Depending on the instrument's model version, there may be several **iConnect** connectors.

- 2 Leave the adapter cable plugged in to protect the connector inside the instrument (1) against mechanical impact.

Connecting the 854 iConnect to the adapter cable

Make sure that the mini USB adapter cable is connected to the instrument.

The 854 iConnect can also be connected while the instrument is switched on.

- 1 Plug the plug of the 854 iConnect (3) into the socket of the mini USB adapter cable (2). Observe the correct orientation (markings).

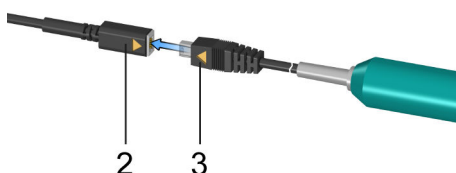


Figure 17 Plugging in the 854 iConnect

As soon as the instrument is switched on, the 854 iConnect is detected automatically and entered as measuring input into the device properties.

Connecting the electrode

The 854 iConnect is used as measuring input for iTrodes (electrodes with integrated memory chip).

Connect the electrode as follows:

- 1** Remove the protective cap of the 854 iConnect.

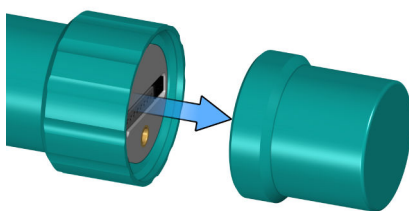


Figure 18 Removing the protective cap

- Align the guide pin (5) of the electrode with the recess in the 854 iConnect (4).

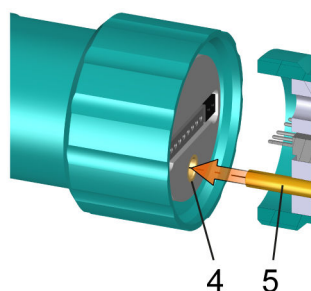


Figure 19 Aligning the guide pin

- 3** Attach the electrode to the 854 iConnect.

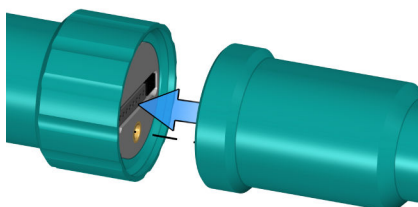


Figure 20 Attaching the electrode

Tighten the screw cap by hand.



Mount the protective cap again as soon as the 854 iConnect is not in use anymore and no electrode is connected.

The 854 iConnect can also be removed while the instrument is switched on.

-

Figure 21 Unplugging the 854 iConnect

- 

Position the mini USB adapter cable in such a way that it cannot be removed by accident.



For further information on the 854 iConnect, see *Manual iConnect 854*, article number 8.854.8002.

4.5.6 Differential potentiometry

Potentiometric measurements with high-ohm measuring chains can be disrupted by electrostatic and electromagnetic fields in media with low conductivity. Use our 6.0229.100 Solvotrode or other special electrodes for pH measurements in organic solvents. If no reliable measurements are possible with these, then a 6.5104.030 (230 V) or 6.5104.040 (115 V) differential amplifier can be used. The differential amplifier is connected to the high-ohm measuring input (**Ind.**).

5 Working with the exchange unit

The exchange unit (806 Exchange Unit) has an integrated data chip that makes it possible to store data about the exchange unit and for the reagent. The data is edited in the Touch Control or in the PC software. The start-up of the exchange unit is described in the manual for the exchange unit.

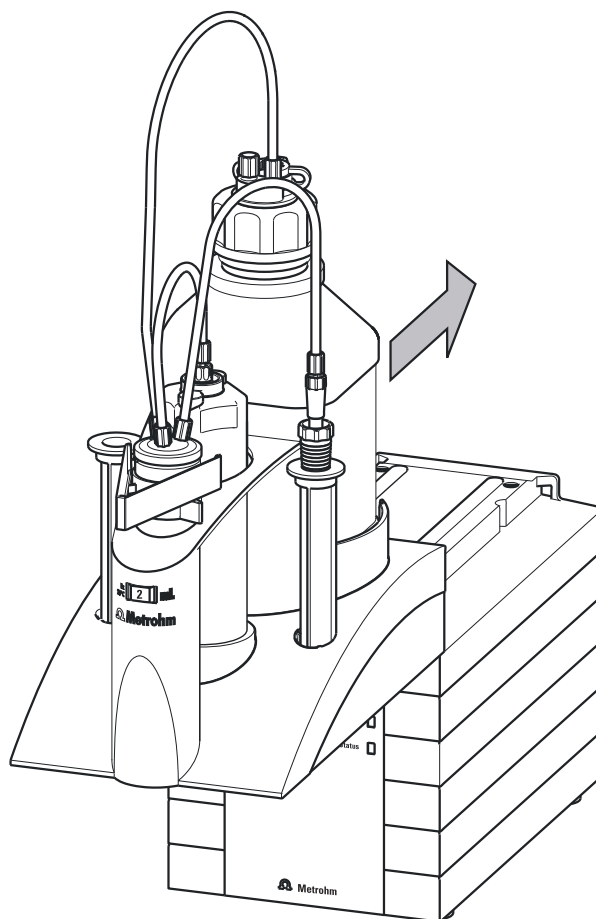


Figure 22 Attaching the exchange unit

Proceed as follows to attach the exchange unit:

- 1** Attach the exchange unit from the front onto the 888 Titrand and push it all the way to the rear.

It must snap in audibly.

If the exchange unit is attached correctly, its initialization is activated by a microswitch which is triggered by the guide bolts of the exchange unit. The exchange unit is recognized and the data is read out automatically from the data chip. The 888 Titrand carries

out an automatic rotation of the flat stopcock and then returns it to the exchange position (dosing position). The **Status** LED will be continuously illuminated once this has been accomplished.

The following table contains a summary of which operating statuses of the internal dosing device are displayed by the **Status** LED:

Status of the "Status" LED	Description
off	No exchange unit is attached.
constant illumination	The exchange unit has been correctly attached and recognized and can now be used for dosing and titration. The flat stopcock is in the exchange position, i.e. the exchange unit can be removed.
slow flashing	▪ The exchange unit is currently being used for dosing or filling. ▪ An intelligent exchange unit has been attached and the data on the integrated data chip is currently either being read out or written.
rapid flashing	Error on the dosing drive, consult the "Troubleshooting" chapter.

6 Operation and maintenance

6.1 General notes

6.1.1 Care

The 888 Titrande requires appropriate care. Excess contamination of the instrument may result in functional disruptions and a reduction in the service life of the otherwise sturdy mechanics and electronics.

Spilled chemicals and solvents should be removed immediately. Above all, the plug connections on the rear of the instrument (in particular the power socket) should be protected from contamination.



CAUTION

Although this is extensively prevented by design measures, the power plug should be unplugged immediately if aggressive media have penetrated the inside of the instrument, so as to avoid serious damage to the instrument electronics. In such cases, Metrohm Service must be informed.

6.1.2 Maintenance by Metrohm Service

Maintenance of the 888 Titrande is best carried out as part of an annual service, which is performed by specialist personnel of the Metrohm company. A shorter maintenance interval may be necessary if you frequently work with caustic and corrosive chemicals.

Metrohm Service offers every form of technical advice for maintenance and service of all Metrohm instruments.

7 Troubleshooting

7.1 General

Problem	Cause	Remedy
The "On" LED is not illuminated, even though the instrument is connected to the power supply.	<i>The Touch Control or the computer has not been switched on yet or the plugs are not correctly plugged in.</i>	1. Check the plug connections. 2. Switch on the Touch Control or the computer.
It is not possible to attach the exchange unit.	<i>The flat stopcock of the exchange unit is not in the exchange position.</i>	Move the green switching lever to the right until it stops.
	<i>The piston rod in the exchange unit is not in the correct position.</i>	Move the piston rod into the correct position (see the manual for the exchange unit).
The exchange unit can not be removed and the "Status" LED is flashing slowly.	<i>The exchange unit is currently being used for dosing or filling.</i>	▪ Wait until the procedure has been completed. ▪ Cancel the procedure manually.
Die "Status" LED does not light up, even though an exchange unit is attached.	<i>The exchange unit has not been attached correctly.</i>	Remove the exchange unit and then attach it once again (it must snap in audibly). The LED flashes while data is read out from an intelligent exchange unit (806 Exchange Unit) and lights up constantly if the exchange unit has been recognized correctly.
The "Status" LED flashes rapidly.	<i>The dosing drive is overloaded because the flat stopcock is jammed.</i>	1. Switch off the Touch Control or exit the PC software. 2. Check whether the exchange unit can be removed. a. If not, move the green switching lever to the right until it stops. 3. Attempt once more to remove the exchange unit; perform maintenance on it afterwards (see the manual for the exchange unit).
	<i>The dosing drive is overloaded because the piston is jammed.</i>	1. Switch the control instrument off and then back on again.

Problem	Cause	Remedy
		- Remove and clean the exchange unit (see the chapter in the manual for the exchange unit, "Care and upkeep"). - Contact your local Metrohm Service department if necessary.
	<i>The data of the exchange unit can no longer be read.</i> <i>The data chip is damaged, either mechanically or by chemical action.</i>	- Contact your local Metrohm Service department to have the data chip replaced. - If necessary, remove the data chip yourself so that the exchange unit can continue to be used in the meantime.

7.2 SET titration

Problem	Cause	Remedy
The titration will not be finished.	<i>The minimum dosing rate is too low.</i>	Select the user-defined titration rate and increase the minimum rate (see manual/help of the software used).
	<i>The stop criterion is unsuitable.</i>	Adjust the control parameters (see manual/help of the software used): - Increase the stop drift. - Select a short delay time.
The sample is over-titrated.	<i>The control parameters are unsuitable.</i>	Adjust the control parameters (see manual/help of the software used): - Select Titration rate = slow. - Select the user-defined titration rate and increase the control range. - Select the user-defined titration rate and reduce the maximum rate. - Select the user-defined titration rate and reduce the minimum rate. - Stir faster. - Arrange the electrode and buret tip to an optimum.
	<i>The electrode responds too slowly.</i>	Replace the electrode.
The titration time is too long.	<i>The control parameters are unsuitable.</i>	Adjust the control parameters (see manual/help of the software used): Select Titration rate = optimal or fast.

8 Appendix

8.1 Remote interface

The 6.2148.010 Remote Box allows devices to be controlled which cannot be connected directly to the MSB interface of the Titrande.

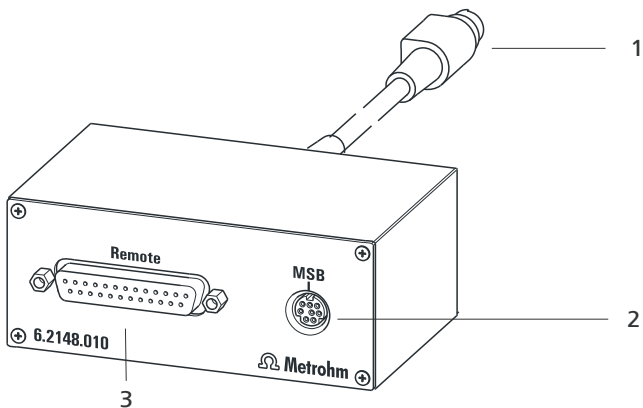


Figure 23 Connectors of the Remote Box

- | | |
|--|---|
| 1 Cable
For connecting to the Titrande. | 2 MSB connector
Metrohm Serial Bus. For connecting external dosing devices or stirrers. |
| 3 Remote connector
For connecting instruments with a remote interface. | |

8.1.1 Pin assignment of the remote interface

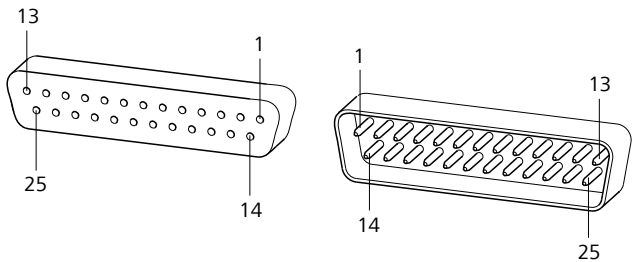


Figure 24 Pin assignment of remote socket and remote plug

The above figure of the pin assignment applies for all Metrohm instruments with 25-pin D-Sub remote connector.

Assignment	Pin No.	Function*
Output 8	6	
Output 9	7	
Output 10	8	
Output 11	13	
Output 12	19	
Output 13	20	
0 volts / GND	14	
+5 volts	15	
0 volts / GND	25	

* Signal activated only for operation with Touch Control.

Table 2 Explanation of the individual functions

Function	Explanation
Start	The current method is started at the time of activation. $t_{\text{pulse}} > 100 \text{ ms}$
Stop	The current method is canceled (Stop) at the time of activation. $t_{\text{pulse}} > 100 \text{ ms}$
Quit	The current command in the determination run will be canceled at the time of activation. $t_{\text{pulse}} > 100 \text{ ms}$
Ready	The instrument is ready to receive a start signal.
Conditioning OK	The line is set when Conditioning with SET titration and KFT titration is at OK. The line remains set until the determination is started with [START] .
Determination	The instrument performs a data-generating determination.
EOD	End of Determination. Pulse ($t_{\text{pulse}} = 200 \text{ ms}$) after a determination or after a buffer/standard solution during calibration using a Sample Processor.
Error	The line is set for error message display.

Function	Explanation
Warning	The line is set for warning message display.

9 Technical specifications

9.1 Measuring interface

The 888 Titrande has one galvanically isolated measuring interface.

The measuring cycle is 100 ms for all measuring modes.

9.1.1 Potentiometry

One high-ohm measuring input (**Ind.**) for pH, metal or ion-selective electrodes and one measuring input (**Ref.**) for separate reference electrodes.

Input resistance $> 1 \cdot 10^{12} \Omega$

Offset current $< 1 \cdot 10^{-12} \text{ A}$ (under reference conditions)

Measuring mode
pH

Measuring range $-13 \text{ to } +20 \text{ pH}$

Resolution 0.001 pH

Measuring accuracy $\pm 0.003 \text{ pH}$
(± 1 digit, without sensor error, under reference conditions)

Measuring mode
U

Measuring range $-1,200 \text{ to } +1,200 \text{ mV}$

Resolution 0.1 mV

Measuring accuracy $\pm 0.2 \text{ mV}$
(± 1 digit, without sensor error, under reference conditions)

9.1.2 Temperature

A measuring input (**Temp.**) for temperature sensors of the Pt1000 or NTC type with automatic temperature compensation.

R (25 °C) and B value can be configured for NTC sensors.

Measuring range

Pt1000 $-150 \text{ to } +250 \text{ °C}$

NTC $-5 \text{ to } +250 \text{ °C}$
(R (25 °C) = 30,000 Ω and B (25/50) = 4,100 K)

Resolution

Pt1000 0.1 °C

9.2 Internal dosing device

<i>Cylinder volume of the exchange unit</i>	1 mL, 5 mL, 10 mL, 20 mL or 50 mL
<i>Resolution</i>	20,000 steps per cylinder volume

9.3 Power connection

<i>Supply voltage</i>	100–240 V ($\pm 10\%$)
<i>Frequency</i>	50–60 Hz ($\pm 3\%$)
<i>Power consumption</i>	Maximum 45 W
<i>Fuse</i>	Electronic overload protection

9.4 Ambient conditions

<i>Automatic interior temperature monitoring</i>	
<i>Nominal function range</i>	+5 to +45 °C at max. 80% relative humidity, non-condensing
<i>Storage</i>	+5 to +45 °C at max. 80% relative humidity, non-condensing
<i>Altitude / Pressure range</i>	max. 2,000 m.a.s.l. sea level / min. 780 mbar
<i>Overvoltage category</i>	II
<i>Pollution degree</i>	2

Connection of a maximum of 4 Remote Boxes. Remote Boxes can be used to actuate and monitor external devices.

6.2151.000 controller cable	15
685 Dosimat plus	18
700 Dosino	18
800 Dosino	18
801 Stirrer	19
803 Ti Stand	19
804 Ti Stand	19
805 Dosimat	18

ADD	4
Ambient conditions	45

Balance	23
Barcode reader	
Connect	25

Calibration mode	
CAL	4
Computer	
Connect	15
Connect	
Balance	23
Barcode reader	25
Computer	15
Dosing device	18
MSB devices	17
PC keyboard	24
Power grid	14
Printer	22
Remote Box	20
Stirrer	19
Titration stand	19
Touch Control	13
USB hub	22
Connector	
MSB	2
USB	2
Controller	
Connector	11

DET	3
Device description	2
Device software	
Update	2
Differential potentiometry	32

Dosing command	3
ADD	4
EMPTY	4
PREP	4
Dosing device	
Connect	18
Driver software	
Install	15

Electrode	
Connect	26
Electrostatic charge	9
EMPTY	4
Exchange unit	33

Humidity 45

Installation	
Driver software	15
Instrument type	11

Keyboard
Connect 24

LED	
On	36
Status	34, 36

Maintenance	35
MEAS	3
Measuring interface	2, 11
Measuring mode	3
MEAS	3
MET	3
Metrohm Serial Bus MSB, see also	
"MSB"	17
MSB	
Connect devices	17
Connector	11
MSB connector	2

Operation	45
Overview of the instrument	10

Overvoltage category 45

PC keyboard	
Connect	24
Pin assignment	39
Power connection	11, 14, 15
PREP	4
Printer	22

Remote	
Interface	39
Pin assignment	39
Remote Box	
Connect	20

Safety instructions	7
Sea level	45
Sensor	
Connect	26
Serial number	11
Service	8
SET	3
Stirrer	
Connect	19
Storage	45
Supply voltage	9
System test	13

Temperature	45
Temperature sensor	
Connect	26
Titrand system	1
Titration mode	3
DET	3
MET	3
SET	3
Titration stand	
Connect	19
Touch Control	
Connect	13

Update	
Device software	2
USB	
Connector	11

888 Titrando