


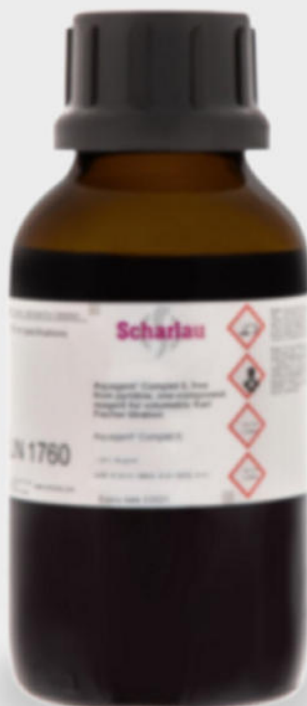

## Application Note AN-K-073

# Volumetric Karl Fischer titration with Scharlau Aquagent® reagents

## Test measurements using Aquagent® Complet 5 and Methanol Fast

This Application Note summarizes a series of test measurements performed with an OMNIS KF Titrator and Karl Fischer reagents Aquagent® Complet 5 and Methanol Fast from Scharlau.

Three series of titer determinations using various water standards were carried out. The results obtained using different water standards were found

to lie in a similar range. The reproducibility of the results was determined to be very good.

Using an OMNIS titration system from Metrohm and the Scharlau Karl Fischer reagents, titer determinations can be carried out quickly without any decline in the reproducibility of results.

## STANDARDS

Three different water standards have been used for the tests performed in this study:

1. Water standard with a water content of approximately 10.0 mg/g («water standard 10»)
2. Sodium tartrate dihydrate with a water content of approximately 15.7%
3. Deionized water

## EXPERIMENTAL

A 10-fold titer determination was carried out with both water standards and the deionized water.

The sample sizes were varied for water standard 10 (between 0.5 g and 4.0 g) as well as for the sodium tartrate dihydrate (between 0.077 g and 0.114 g). A constant sample size of 25 µg was used for the

deionized water.

The water standard 10 was added with a glass syringe. To add the sodium tartrate dihydrate, a weighing boat (6.2412.000) was used. The deionized water was injected into the titration cell with a microliter syringe.

## RESULTS

The following table shows the results of three titer determination series using using Aquagent® Complet

5 and Methanol Fast reagents from Scharlau.

**Table 1.** Results of the titer determination series (n = 10) with three water standards.

| Standard | Titer in mg/mL | s(abs) in mg/mL | s(rel) in % |
|----------|----------------|-----------------|-------------|
| 1        | 5.3936         | 0.02248         | 0.09        |
| 2        | 5.3781         | 0.00485         | 0.16        |
| 3        | 5.3459         | 0.00873         | 0.42        |

## CONCLUSION

The titer determinations were both fast and reproducible. The relative standard deviations were very low, especially for the water standard 10 and the sodium tartrate dihydrate.

Methanol Fast contains additives to accelerate the titration, therefore it is recommended to use the method parameters suitable for two-component reagents (Table 2).

**Table 2.** List of suitable method parameters for two-component reagents in OMNIS.

| Parameter             | Value      |
|-----------------------|------------|
| Dynamics              | 300 mV     |
| Max. rate             | max        |
| Min. volume increment | min        |
| I <sub>pol</sub>      | 50 $\mu$ A |
| EP                    | 250 mV     |

## CONTACT

Metrohm UK & Ireland  
Evenwood Close  
WA71LZ Runcorn

[info@metrohm.co.uk](mailto:info@metrohm.co.uk)

## CONFIGURATION



### OMNIS Titrator KF

The OMNIS Titrator KF offers you the complete package for volumetric Karl Fischer titration. Included in the package is the OMNIS Basic Titrator with magnetic stirrer for potentiometric end point titration, the function license for KFT with conditioning, the OMNIS Solvent Module and the complete accessories for volumetric Karl Fischer titration.

Benefit from the unique user-friendliness of an automatic start of titration after sample addition and maximum safety thanks to contact-free reagent handling with the 3S-Liquid Adapter and OMNIS Solvent Module.