



Application Note AN-NIR-022

# Quality Control of Gasoline

Rapid determination of RON, MON, AKI, aromatic content, and density

In recent years, there has been a significant push to reduce the environmental impacts of fuels through improvements to fuel quality. This requires engines to be more efficient, along with increasing the octane content of fuel so higher compression engines can be utilized. The determination of key quality parameters of gasoline, namely research octane number (RON, ASTM D2699-19), motor octane number (MON, ASTM D2700-19), anti knock index (AKI), aromatic content

(ASTM D5769-15), and density, conventionally requires several different analytical methods, which are laborious and need trained personnel. This application note demonstrates that the XDS RapidLiquid Analyzer, operating in the visible and near-infrared spectral region (Vis- NIR), provides a cost-efficient and fast solution for the multiparameter analysis of gasoline.

## EXPERIMENTAL EQUIPMENT

Gasoline samples were measured with the XDS RapidLiquid Analyzer (RLA) in transmission mode over the full wavelength range (400–2500 nm). Reproducible spectrum acquisition was achieved using the built-in temperature controlled sample holder. For convenience, disposable vials with a path length of 8 mm were used, which made a cleaning procedure unnecessary. The Metrohm software package Vision Air Complete was used for data acquisition and prediction model development.



**Figure 1.** XDS RapidLiquid Analyzer and 8 mm disposable vial filled with a gasoline sample.


**Table 1.** Hardware and software equipment overview

| Equipment                                     | Metrohm number |
|-----------------------------------------------|----------------|
| XDS RapidLiquid Analyzer                      | 2.921.1410     |
| Disposable vials, 8 mm diameter, transmission | 6.7402.000     |
| Vision Air 2.0 Complete                       | 6.6072.208     |


## RESULTS

The obtained Vis-NIR spectra (**Figure 2**) were used to create prediction models for the determination of several key fuel parameters. The quality of the prediction models was evaluated using correlation

diagrams, which display a correlation between the Vis-NIR prediction and primary method values. The respective figures of merit (FOM) display the expected precision of a prediction during routine analysis.

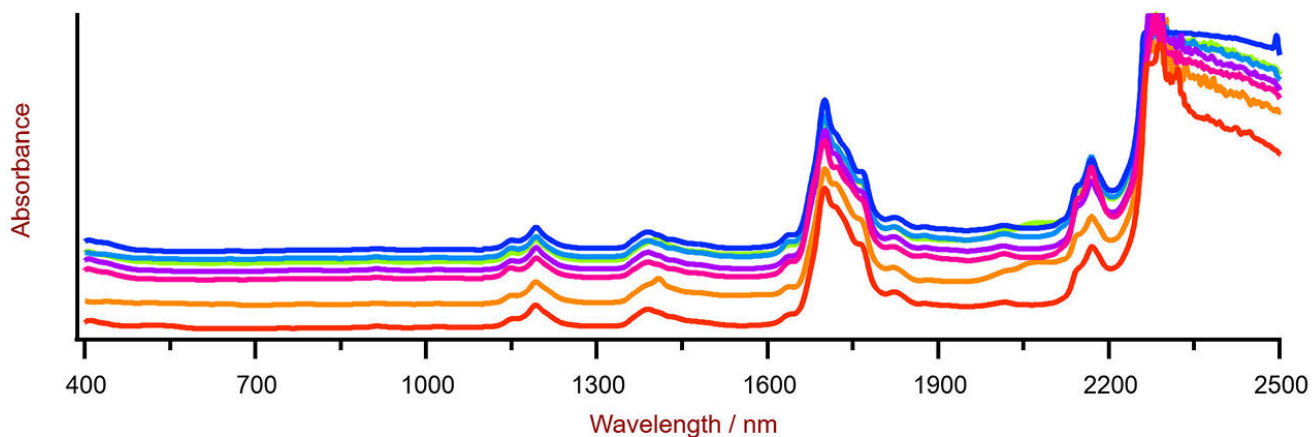


**Figure 2.** This selection of gasoline Vis-NIR spectra was obtained using a XDS RapidLiquid Analyzer and 8 mm disposable vials. For display reasons a spectra offset was applied.

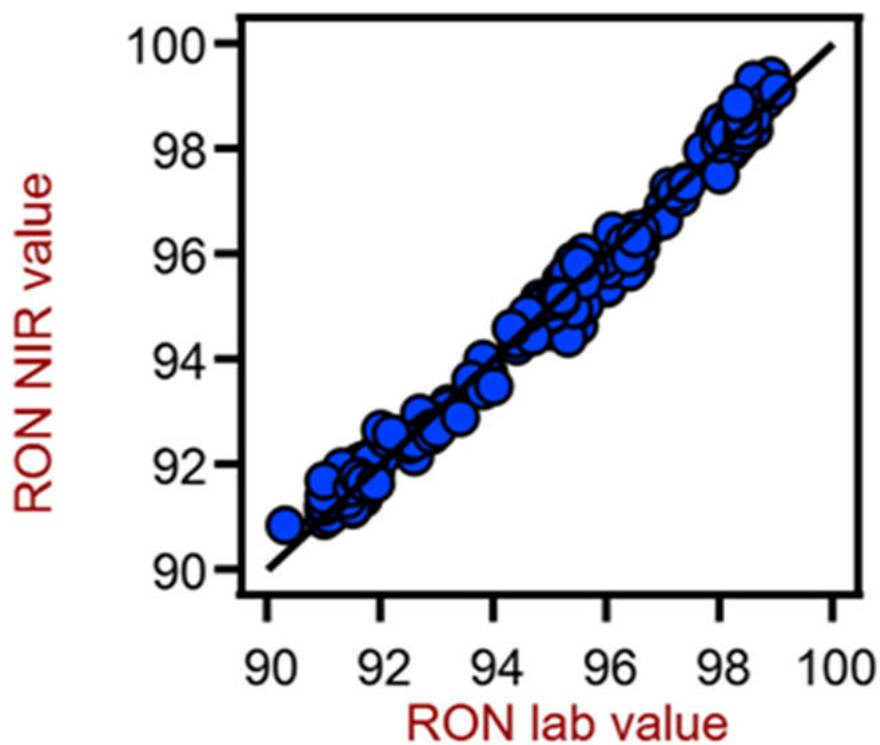

**Figure 3.** Correlation diagram for the prediction of the RON value in gasoline using a XDS RapidLiquid Analyzer. The reference lab values were determined according to CFR engine tests under controlled conditions.

**Table 2.** Figures of merit for the prediction of the RON value in gasoline using a XDS RapidLiquid Analyzer.

| Figures of merit                   | Value |
|------------------------------------|-------|
| $R^2$                              | 0.989 |
| Standard error of calibration      | 0.26  |
| Standard error of cross-validation | 0.29  |

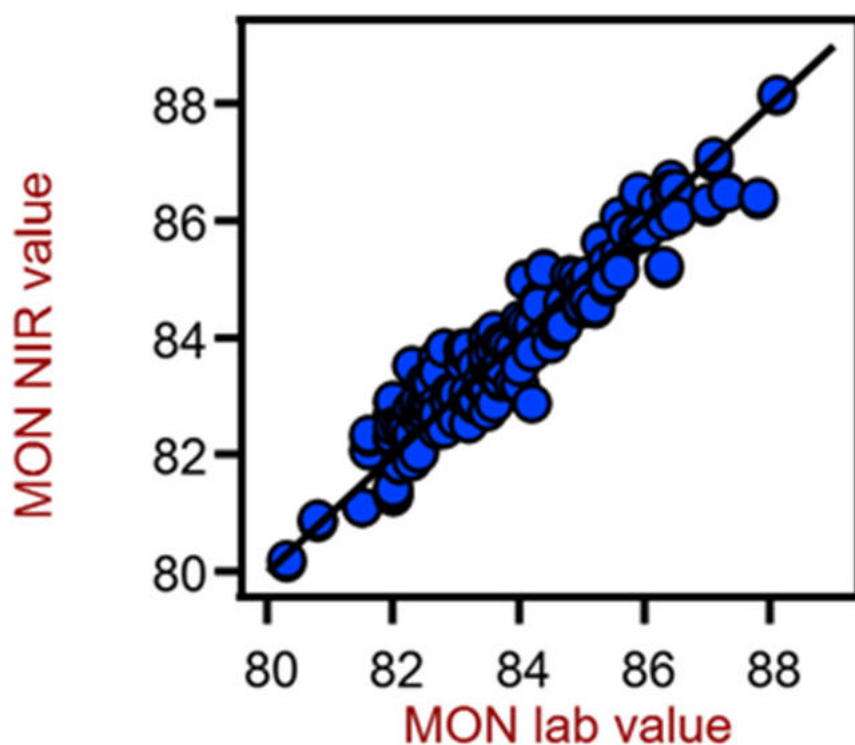


**Figure 4.** Correlation diagram for the prediction of the MON value in gasoline using a XDS RapidLiquid Analyzer. The reference lab values were determined according to CFR engine tests under controlled conditions.

**Table 3.** Figures of merit for the prediction of the MON value in gasoline using a XDS RapidLiquid Analyzer.

| Figures of merit                   | Value |
|------------------------------------|-------|
| $R^2$                              | 0.889 |
| Standard error of calibration      | 0.50  |
| Standard error of cross-validation | 0.53  |


## RESULTS

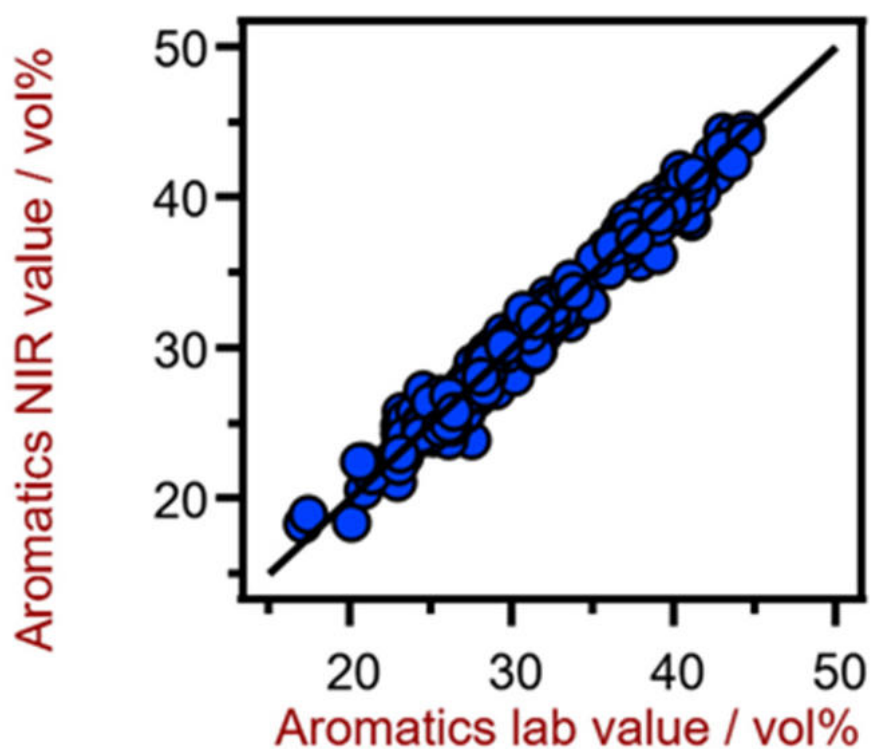

**Figure 5.** Correlation diagram for the prediction of the aromatics content in gasoline using a XDS RapidLiquid Analyzer. The lab values were determined with gas chromatography/mass spectrometry techniques.

**Table 4.** Figures of merit for the prediction of the aromatics content in gasoline using a XDS RapidLiquid Analyzer.


| Figures of merit                   | Value     |
|------------------------------------|-----------|
| $R^2$                              | 0.974     |
| Standard error of calibration      | 0.97 vol% |
| Standard error of cross-validation | 1.07 vol% |

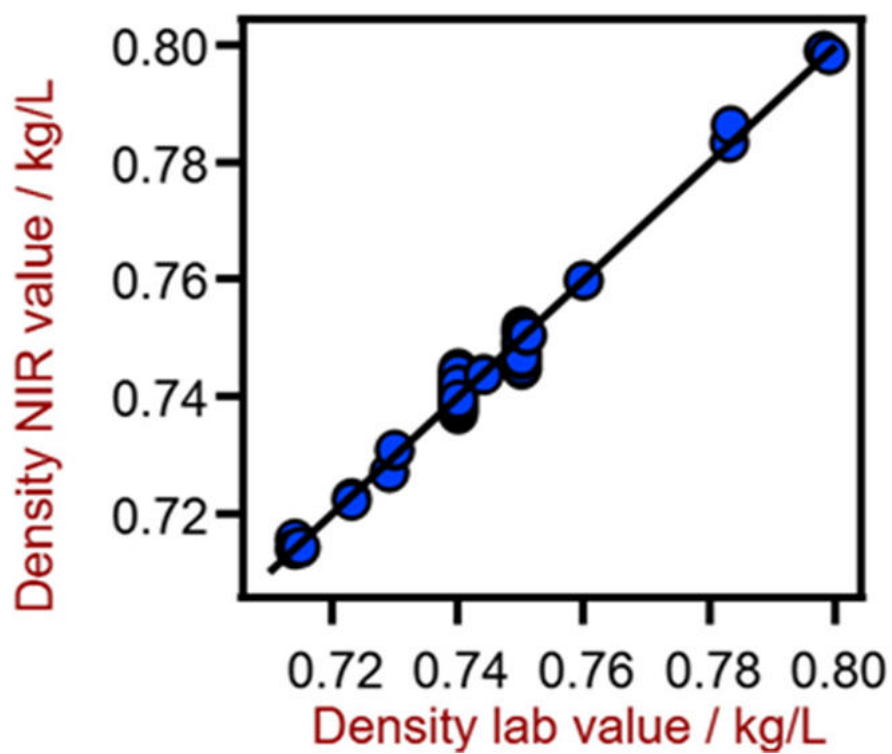

**Figure 6.** Correlation diagram for the prediction of gasoline density using a XDS RapidLiquid Analyzer. The lab values were determined using a density meter.

**Table 5.** Figures of merit for the prediction of gasoline density using a XDS RapidLiquid Analyzer.

| Figures of merit                   | Value       |
|------------------------------------|-------------|
| $R^2$                              | 0.973       |
| Standard error of calibration      | 0.0021 kg/L |
| Standard error of cross-validation | 0.0023 kg/L |

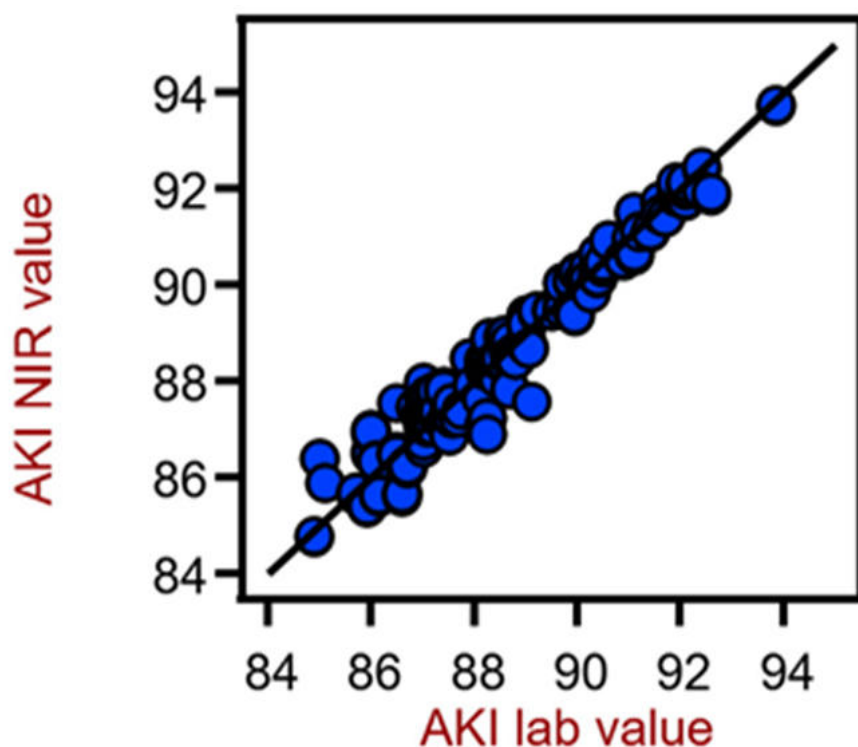

**Figure 7.** Correlation diagram for the prediction of AKI value in gasoline using a XDS RapidLiquid Analyzer. The reference lab values were determined according to CFR engine tests under controlled conditions.

**Table 6.** Figures of merit for the prediction of the AKI value in gasoline using a XDS RapidLiquid Analyzer.

| Figures of merit                   | Value |
|------------------------------------|-------|
| $R^2$                              | 0.945 |
| Standard error of calibration      | 0.45  |
| Standard error of cross-validation | 0.46  |

## CONCLUSION

This application note shows the feasibility of NIR spectroscopy for the analysis of RON, MON, AKI, aromatic content, and density. In comparison to wet

chemical methods (Table 7), the time to result is a major advantage of NIR spectroscopy, since a single measurement is performed within one minute.

**Table 7.** Time to result with conventional testing methods

| Parameter        | Method             | Time to result        |
|------------------|--------------------|-----------------------|
| RON              | CFR engine test    | 30 minutes per sample |
| MON              | CFR engine test    | 30 minutes per sample |
| AKI              | CFR engine test    | 30 minutes per sample |
| Aromatic content | Gas Chromatography | 45 minutes per sample |

To view the information for all key parameters and to get the latest information, please check out our precalibrations:

[Pre-calibrations](#)

## CONTACT

Metrohm AG  
Ionenstrasse  
9100 Herisau

[info@metrohm.com](mailto:info@metrohm.com)



### NIRS XDS RapidLiquid Analyzer

Rapid, precise analyses of liquids and suspensions of all types.

The NIRS XDS RapidLiquid Analyzer enables rapid, precise analyses of liquid formulations and substances. Precise measurement results at the push of a button make the NIRS XDS RapidLiquid Analyzer an equally reliable and simple solution for quality monitoring in laboratories and processes. The samples are transferred to quartz cuvettes designed for multiple use or disposable glass vials; a tempered sample compartment ensures reproducible analysis conditions and thus accurate measurement results.



## Vision Air 2.0 Complete

Vision Air - Universal spectroscopy software.

Vision Air Complete is a modern and simple-to-operate software solution for use in a regulated environment.

Overview of the advantages of Vision Air:

- Individual software applications with adapted user interfaces ensure intuitive and simple operation
- Simple creation and maintenance of operating procedures
- SQL database for secure and simple data management

The Vision Air Complete version (66072208) includes all applications for quality assurance using Vis-NIR spectroscopy:

- Application for instrument and data management
- Application for method development
- Application for routine analysis

Additional Vision Air Complete solutions:

- 66072207 (Vision Air Network Complete)
- 66072209 (Vision Air Pharma Complete)
- 66072210 (Vision Air Pharma Network Complete)