



Application Note AN-V-127

Fe(II) in iron sucrose injection (USP)

Polarographic determination of limit of iron(II) according to USP–NF

Iron sucrose injection is a medical product commonly used for the treatment of iron deficiency anemia. Iron sucrose is a dark brown liquid which contains sucrose and iron(III) hydroxide in an aqueous solution. Once administered to the blood stream the iron (III) is stored in the protein ferritin where it is available for the production of the protein hemoglobin as a part of the red blood cells, which are essential for the transport of oxygen.

As a medical product, iron sucrose is subject to strict controls. Among other tests, the U.S. Pharmacopeia (USP) requires to monitor the limit of Fe(II) in the iron

sucrose injection solution by polarography. The benefit of polarography is that Fe(II) and Fe(III) show signals at different potentials, and therefore an easier determination of Fe(II) without a previous separation of the two oxidation states is possible.

The 884 Professional VA together with the viva software allows a straightforward determination of the Fe(II) content of iron sucrose injection solution following the requirements of the USP. The Fe(II) content is automatically calculated and stored in a database together with all relevant determination and calculation parameters.

EXPERIMENTAL

The concentration of Fe(II) is determined in iron sucrose injection solutions using polarography. Sodium acetate supporting electrolyte is deaerated for 5 minutes. Then the sample is added, and the polarogram is recorded using the parameters listed in Table 1.

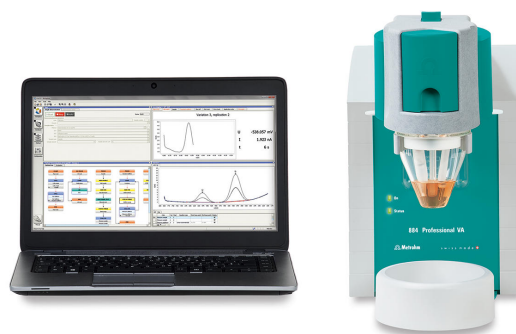


Figure 1. 884 Professional VA.

Table 1. Parameters

Parameter	Setting
Working electrode	SMDE
Mode	DP – Differential Pulse
Start potential	-0.1 V
End potential	-1.75 V
Peak potential Fe(III) -> Fe(II)	-0.75 V
Peak potential Fe(II) -> Fe ⁰	-1.4 V

ELECTRODES

- Working electrode: Multi-Mode Electrode pro with standard glass capillaries
- Reference electrode: Ag/AgCl/KCl (3 mol/L) reference electrode with electrolyte vessel.
Bridge electrolyte: KCl (3 mol/L)
- Auxiliary electrode: Platinum rod electrode

Two signals are recorded, one for the reduction of $\text{Fe(III)} \rightarrow \text{Fe(II)}$, and the second for the reduction of

$\text{Fe(II)} \rightarrow \text{Fe}^0$. The concentration of Fe(II) is calculated as follows:

$$w(\text{Fe}^{2+}) = \left[1 - \frac{2}{R} \right] \times w(\text{Fe}(\text{total})) \quad [\%w/v]$$

in which R is defined as:

$$R = \frac{\text{peak height } (\text{Fe}^{2+} \rightarrow \text{Fe}^0)}{\text{peak height } (\text{Fe}^{3+} \rightarrow \text{Fe}^{2+})}$$

RESULTS

The total iron concentration $w(\text{Fe}(\text{total}))$ is determined in a separate analysis by AAS (atomic absorption spectroscopy).

The calculation in this application can be done automatically in the **viva** software.

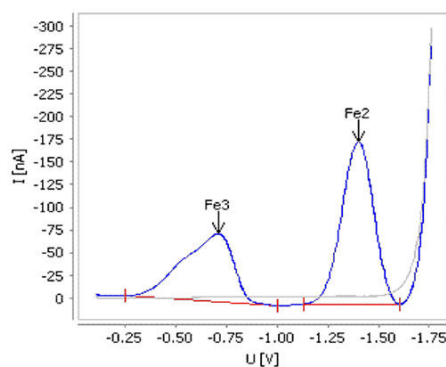


Figure 2. Determination of iron in iron sucrose injection

Table 2. Result

Sample	Fe(II) concentration
Iron sucrose injection	0.33%

REFERENCE

United States Pharmacopeia USP 39–NF 34

Internal references: AW CH4-0452-112006; AW VA CH4-0565-092017

CONTACT

Metrohm SA
1 Bridle Close
2052 Woodmead

sales@metrohm.co.za

CONFIGURATION



884 Professional VA manual for Multi-Mode Electrode (MME)

884 Professional VA manual for Multi-Mode Electrode (MME) is the entry-level instrument for high-end trace analysis with voltammetry and polarography with the Multi-Mode Electrode pro or the scTRACE Gold or the Bismuth drop electrode. The proven Metrohm electrode methods in combination with a high-performance potentiostat/galvanostat and the extremely flexible viva software open up new perspectives for the determination of heavy metals. The potentiostat with a certified calibrator readjusts itself automatically before each measurement, thus guaranteeing maximum precision.

Determinations with rotating disc electrodes can also be performed with the instrument, e.g. determinations of organic additives in electroplating baths with "Cyclic Voltammetric Stripping" (CVS), "Cyclic Pulse Voltammetric Stripping" (CPVS), and chronopotentiometry (CP). The replaceable measuring head enables rapid changes between the various applications with different electrodes.

The **viva** software is required for control, data collection, and evaluation.

The 884 Professional VA manual for MME is supplied with extensive accessories and a measuring head for the Multi-Mode Electrode pro. Electrode set and **viva** license need to be ordered separately.



VA electrode equipment with Multi-Mode Electrode pro for Professional VA instruments

Complete electrode set for polarographic and voltammetric determinations. Includes Multi-Mode Electrode pro, reference electrode, platinum auxiliary electrode, measuring vessel, stirrer, electrolyte solution and additional accessories for setting up and operating the Multi-Mode Electrode.