



## Application Note AN-T-208

# Nicotine in e-liquids

## Reliable and affordable determination by potentiometric titration

The vaping and electronic cigarette industries have grown impressively in the past decade. Usage among youths has increased from around 1% in 2011 to 10.5–27.5% in 2019 (pre-teens vs. older teenagers) mainly due to the vast array of flavor options available (Truth Initiative, 2020). The mixtures used in these products are usually called «e-liquid», «e-fluid», or «e-juice». To ensure the quality of these e-liquids, testing the most important quality parameters is required. One important quality control parameter is the nicotine content available in these products. Nicotine in tobacco is usually determined by gas

chromatography or liquid chromatography. Aqueous acid base titration is a much more affordable alternative for this determination. As e-liquids do not contain other components which might interfere with the titration, the aqueous acid base titration presented in this Application Note can be applied for nicotine determination.

This method is an affordable and reliable way to determine the nicotine content in e-liquids and their nicotine starting material, ensuring the quality of these products.

## SAMPLE AND SAMPLE PREPARATION


Nicotine starting material for e-liquids as well as e-liquids are analyzed. No sample preparation is

required.

## EXPERIMENTAL

The analyses are carried out on a 905 Titrando system with a rod stirrer and a Unitrode easyClean for indication of the equivalence point.

A suitable amount of sample is transferred into a disposable beaker and deionized water is added. The solution is stirred to ensure complete dissolution and mixing. Afterwards, the solution is titrated with standardized hydrochloric acid until after the first equivalence point is reached.

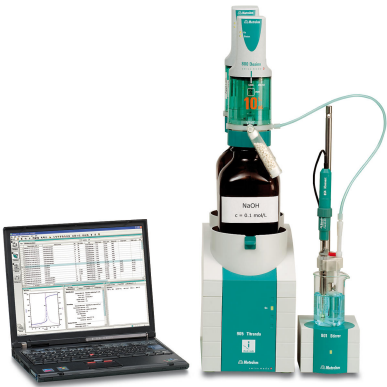

**Figure 1.** Titration system consisting of a 905 Titrando, a rod stirrer, and a Unitrode easyClean. The data are recorded and evaluated by tiamo.


## RESULTS

Steep and smooth titration curves are obtained for all analyses. An example titration curve is displayed in **Figure 2**. The automated analysis leads to

reproducible results with low RSDs as shown in **Table 1**.

**Table 1.** Results of the nicotine determination by aqueous titration in nicotine starting materials as well as in various e-liquids (n = 3).

|                            | Mean value / g/L | SD(abs) / g/L | SD(rel) /% |
|----------------------------|------------------|---------------|------------|
| Nicotine starting material | 31.39            | 0.01          | 0.03       |
| E-liquid 1                 | 5.64             | 0.01          | 0.24       |
| E-liquid 2                 | 2.82             | 0.001         | 0.04       |
| E-liquid 3                 | 15.32            | 0.08          | 0.53       |
| E-liquid 4                 | 10.15            | 0.04          | 0.35       |

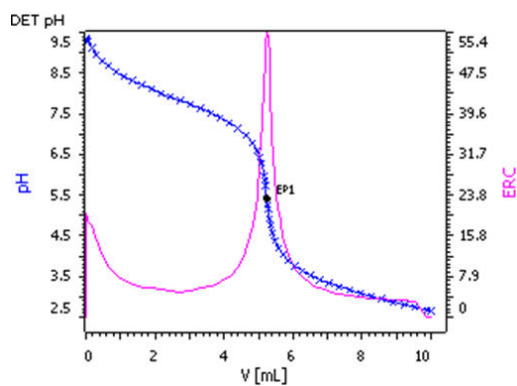

**Figure 2.** Example titration curve for the nicotine determination in an e-liquid.

## CONCLUSION

This method is an affordable and reliable way to determine the nicotine content in e-liquids and their nicotine starting material, ensuring the quality of

these products. Additionally, no harmful chemicals and no sample preparation are required for the determination.

Internal reference: AW TI US1-0073-092018

## CONTACT

143-0006 6-1-1  
null 9

metrohm.jp@metrohm.jp

## CONFIGURATION



### 905 Titrando

Dosino-ドージングシステムを用いた用途のための測定インターフェースを備えた電位差滴定のためのハイエンド滴定装置。

- タイプ800 Dosinoのドージングシステムが4つまで
- 変動滴下量当量点滴定 (DET)、等量滴下当量点滴定 (MET)、終点滴定 (SET)
- イオン選択性電極を用いた測定 (MEAS CONC)
- モニタリング、LQHを備えたドージング機能
- 追加スターラーまたはドージングシステムのための4つのMSBコネクタ
- インテリジェント電極「iTrode」
- USB コネクタ
- OMNISソフトウェア、*tiamo*ソフトウェアもしくはTouch Controlを適用
- GMP/GLP基準およびFDA 基準21 CFR Part 11の要件を満たしています(必要な場合)



### 804 Ti Stand 802 Stirrer

プロペラスターラ 6.1909.010 を備えるロッドスターラ。



### 804 Ti Stand with stand

Titration stand and controller for 802 Rod Stirrer. The 804 Ti Stand together with the optional 802 Rod Stirrer provides an alternative to the magnetic stirrer. Ti Stand with base plate, support rod and electrode holder.



Unitrode easyCleanPt1000 ( 2 m)

easyCleanPt1000pH (2.0 m):

- pH

-

-

easyClean

: c(KCl) = 3 mol / L

: T>80°C: