



Application Note AN-PAN-1013

Online analysis of boric acid in the cooling water of pressurized water reactors

Boric acid is used to absorb neutrons in the primary circuit of pressurized water reactors (PWR) of nuclear reactors, thus controlling the reactor's reactivity. Therefore, near-continuous monitoring of boric acid concentrations is crucial. Boric acid is typically monitored by manual laboratory analysis methods, but these are time-consuming and prone to human error. However, fast, reliable, online analysis is possible with the 2060 TI Process Analyzer.

This Process Application Note discusses the online analysis of boron in nuclear PWRs. The

2060 TI Process Analyzer's adaptive software, IMPACT, automatically switches between various burets, each with a different titrant strength depending on the boric acid concentration to maintain optimal accuracy across the entire measurement range. When integrated with the chemical and volume control system (CVCS), real-time monitoring enables early detection and mitigation of potential boric acid concentration issues, optimizing reactor control for safe and efficient operation.

INTRODUCTION

Approximately 9% of global electricity comes from nuclear energy sources [1]. Pressurized water reactors (PWRs) are one of the most common types of nuclear reactors for electricity generation purposes [1]. The safe and efficient operation of PWRs is critical to ensure a reliable energy supply while also protecting the environment.

In these PWRs, boric acid (B-10 isotope, ^{10}B) is added to the primary coolant to regulate the nuclear reaction. Boron effectively absorbs neutrons, preventing them from sustaining the fission process. By adjusting the concentration of boric acid in the coolant, operators can precisely control the reactor's power output.

Boron is carefully controlled within the primary and secondary circuit (**Figure 1**). While these circuits are designed to be highly contained,

potential risks such as accidents, leaks, or spills could lead to the release of contaminated water into the environment, ultimately impacting nearby water sources.

The boron concentration in the primary coolant varies from 0 to 2,000 mg/L or more, depending on the stage of the fuel cycle [2]. This is significantly higher than the maximum recommended level for drinking water, which is 2.4 mg/L according to the World Health Organization (WHO) [3], and 1 mg/L according to EU standards [4].

The CVCS is responsible for regulating boron concentrations in the reactor coolant. This system carefully adjusts the amount of boric acid added to the primary circuit to maintain optimal reactivity and ensure safe reactor operation.

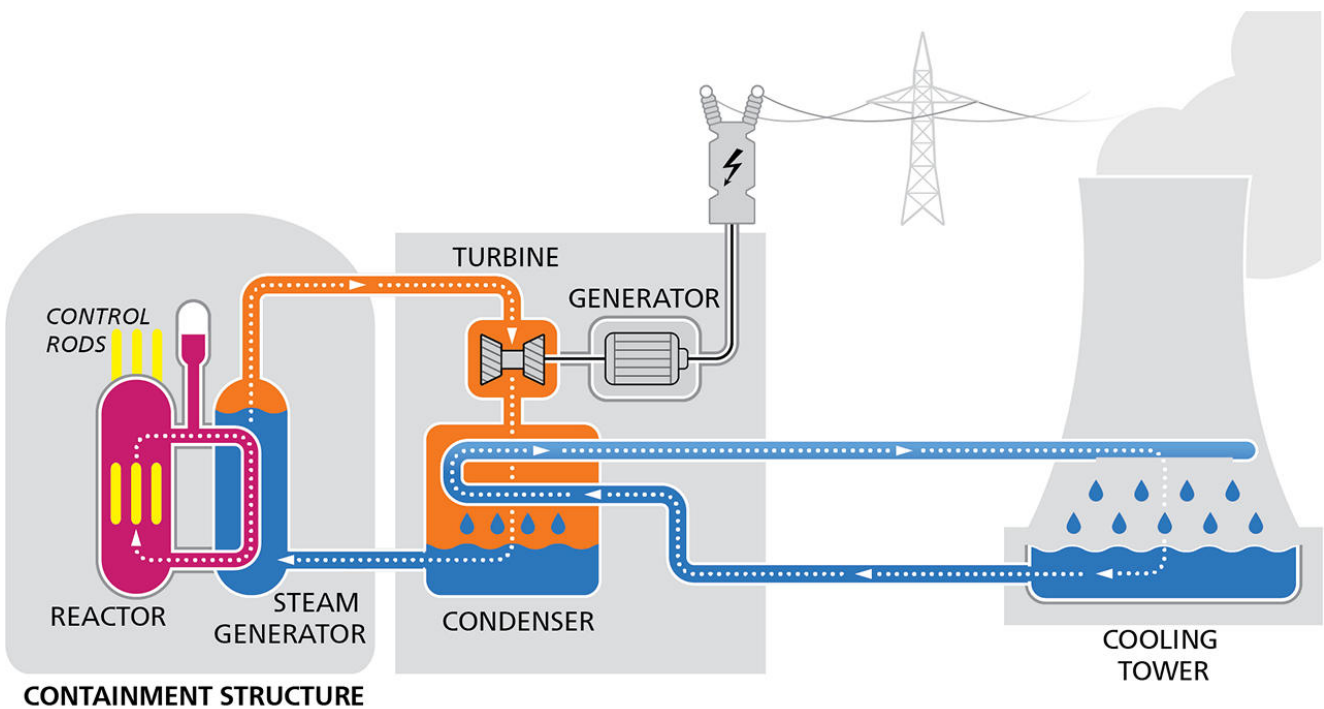


Figure 1. Illustration of the various water circuits in a nuclear reactor (left: primary circuit, center: secondary circuit, right: cooling circuit).

The **2060 TI Process Analyzer (Figure 2)** offers a significant advantage over traditional laboratory testing methods in the nuclear sector. Its advanced titration technique enables continuous, real-time monitoring of boron concentrations in the PWR without the need for manual laboratory testing. Furthermore, the analyzer's self-calibration feature ensures consistent accuracy without

requiring frequent manual adjustments. By seamlessly integrating with nuclear power plant control systems, the **2060 TI Process Analyzer** enables automated reactivity adjustments based on measured boron concentrations. This automation enhances operational efficiency and helps maintain optimal reactor performance.

APPLICATION

Online monitoring of boric acid in cooling water is possible by means of potentiometric titration. The intelligent IMPACT software utilized by the 2060 TI Process Analyzer can automatically

adapt to varying boric acid levels and switch titrant buret concentrations to ensure the highest accuracy is achieved throughout the full measuring range.

Table 1. Typical boric acid concentrations found in pressurized water reactors.

Parameters	[mg/L]
Boron	0–2000

REMARKS

Other process applications related to the water circuits of energy producers include silica, sodium, nickel, zinc, calcium, magnesium, and chloride. Reliable measurements of these critical parameters are possible with the 2060 TI Process Analyzer from Metrohm Process Analytics (**Figure 2**).



Figure 2. The 2060 TI Process Analyzer is suitable to monitor several critical parameters in nuclear pressurized water reactors.

CONCLUSION

The ability to monitor boric acid concentrations within the range of 0–2000 mg/L is particularly valuable in PWRs, where precise control of this parameter is essential for safe and efficient

operation. The 2060 TI Process Analyzer's versatility and accuracy make it a valuable tool for nuclear power plant operators.

REFERENCES

1. *Nuclear Power in the World Today - World Nuclear Association*. <https://world-nuclear.org/information-library/current-and-future-generation/nuclear-power-in-the-world-today> (accessed 2024-08-20).
2. Mesquita, A. Z.; Reis, I. C.; de Almeida, V. F.; et al. Boron-10 Effect on the Reactivity of the IPR-R1 Triga Research Reactor. *Annals of Nuclear Energy* **2019**, *132*, 64–69. DOI:10.1016/j.anucene.2019.04.023
3. *Boron, a key challenge for reverse osmosis systems, successfully treated with LG Chem TFN membranes GWI*. <https://www.globalwaterintel.com/articles/boron-a-key-challenge-for-reverse-osmosis-systems-successfully-treated-with-lg-chem-tfn-membranes-lg-chem> (accessed 2024-08-19).
4. *EU's drinking water standards*. <https://www.lenntech.com/applications/drinking/standards/eu-s-drinking-water-standards.htm> (accessed 2024-08-19).

RELATED APPLICATION NOTES

[AN-PAN-1016 Online analysis of silica in boiler feed water of power plants](#)

[AN-PAN-1032 Monitoring corrosion in power plants with online process analysis](#)

[AN-PAN-1038 Power generation: analysis of the m-number \(alkalinity\) in cooling water](#)

[AN-PAN-1040 Ammonia in cooling water of thermal power plants](#)

[AN-PAN-1042 Online trace analysis of anions in](#)

[the primary circuit of nuclear power plants](#)

[AN-PAN-1043 Online trace analysis of cations in the primary circuit of nuclear power plants](#)

[AN-PAN-1044 Online trace analysis of amines in the alkaline water-steam circuit of power plants](#)

[AN-PAN-1045 Online monitoring of copper corrosion inhibitors in cooling water](#)

[AN-PAN-1056 Online monitoring of sodium in industrial power plants](#)

BENEFITS FOR ONLINE PROCESS ANALYSIS

- **Safer working environment** for employees (nuclear reactor).
- **Fully automated diagnostics** – automatic alarms for when samples are out of specification parameters.
- **Guarantee compliance** with environmental standards.
- **High accuracy** for lower detection limits of boron.



CONTACT

メトロームジャパン株式会
社
143-0006 東京都大田区平
和島6-1-1
null 東京流通センター アネ
ックス9階

metrohm.jp@metrohm.jp

CONFIGURATION



2060 Process Analyzer

2060 Process Analyzerは、無数のアプリケーションに対応するオンライン湿式化学アナライザーです。このプロセスアナライザーは、「ベーシックキャビネット」と呼ばれる中核プラットフォームによって構成される新たなモジュラー式コンセプトを提供するものです。

ベーシックキャビネットは、2つの部分から構成されます。上部はタッチスクリーンと産業用PCを含みます。下部には、実際の分析のためのハードウェアが格納されるフレキシブルな湿式部が含まれます。基本湿式部の容量が分析課題を解決するのに充分でない場合、最も困難なアプリケーションでも解決できる十分なスペースを確保するため、ベーシックキャビネットを4つまでの追加湿式部キャビネットに拡張することが可能です。追加キャビネットは、各湿式部キャビネットを、アナライザーの稼働時間を増加させる内蔵式(非接触式)レベル検出を有する試薬キャビネットと組み合わせるという方法によってコンフィグレーションすることができます。

2060 Process Analyzerは様々な湿式化学技術を提供します: カール フィッシャー滴定、光度測定、直接測定、および標準追加メソッドです。

プロジェクトのすべての要求を満たすべく(もしくはお客様のすべての必要性を満たすため)、頑丈な分析ソリューションを保証するためのサンプルプレコンディショニングシステムをご利用いただくことも可能です。弊社は、冷却や加熱、減圧、脱気、ろ過などのような、いかなるサンプルプレコンディショニングシステムでも提供することができます。