



Application Note AN-RS-029

Trace Detection of Malathion on Corn

Protecting consumer safety with Misa

Malathion is an insecticide widely used on a broad spectrum of plant species. Although classified as having low toxicity, ingestion or acute skin exposure can be dangerous to humans. Several studies have implicated chronic exposure to malathion in the development of certain cancers. Maximum residue limits for malathion have been enacted by the regulatory agencies of several countries: the US Food and Drug Administration sets maximum residue limits at 8 $\mu\text{g/g}$ in foods, while the EU has a

considerably more stringent limit of 20 ng/g . SERS is an accepted method for detection of malathion on fruit and vegetable surfaces. Misa (Metrohm Instant SERS Analyzer), which requires minimal laboratory chemicals and consumables and provides an extremely user-friendly interface, is an excellent SERS solution for trace detection of food adulterants. Misa is a formidable advancement in cost and convenience related to food safety testing and data analysis.

INTRODUCTION

This application note describes a simulated test procedure for detecting malathion sprayed on corn kernels. The assay is based on the

acquisition of SERS-specific spectra for malathion in acetone extracts using Misa and gold nanoparticles (Au NPs).

REFERENCE SPECTRUM AND LIBRARY CREATION

To establish a reference spectrum, a pure malathion standard at 100 $\mu\text{g/mL}$ in ethanol was analyzed using Au NPs. The unique SERS

spectrum shown in **Figure 1** can be used to create a library entry for malathion.

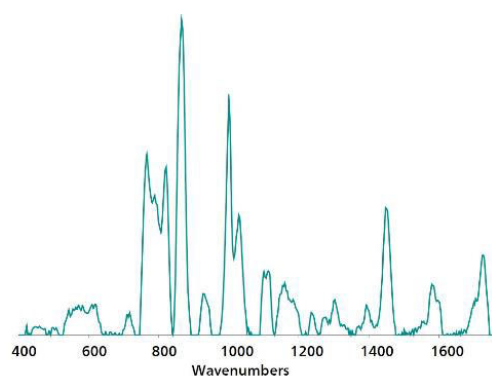


Figure 1. Standard Au NP SERS reference spectrum of malathion.

EXPERIMENT

A stock solution of malathion in acetone was sprayed onto field corn kernels to yield a range of test samples from 1–20 $\mu\text{g/g}$ (concentrations calculated with respect to mass of corn kernels). 0.25 mL of acetone was added to samples in capped glass vials, which were swirled occasionally over a period of 10 minutes to facilitate extraction. At the end of this time, 100 μL of the acetone extract was transferred to a second glass vial and dried on a hot plate. The residue was resuspended in 450 μL of Au NPs and 50 μL of 0.5 mol/L NaCl, the vial was gently shaken to mix, and then immediately placed into the vial attachment on Misa for measurement.



Table 1. Experimental parameters

Instrument		Acquisition	
Firmware	0.9.33	Laser Power	5
Software	Misa Cal V1.0.15	Int. Time	10 s
Misa Vial Attachment	6.07505.040	Averages	10
ID Kit - Au NP	6.07506.440	Raster	ON

RESULTS

Overlaid baseline-corrected spectra acquired for malathion recovered from corn kernels reveal high-resolution malathion detection down to 5 $\mu\text{g/g}$ (**Figure 2**). Note at these low

concentrations, SERS spectra are very sensitive to any other SERS-active moieties present, including organic materials dissolved with the target compound and the SERS substrate itself.

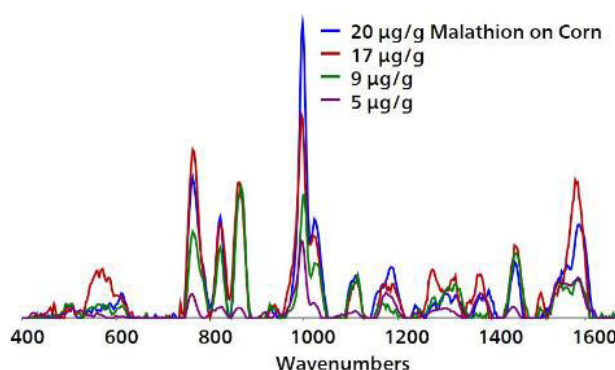


Figure 2. Overlaid baseline-corrected spectra acquired from Au NPs show detection of malathion on field corn kernels to 5 $\mu\text{g/g}$.

FIELD TEST PROTOCOL

Detection of malathion in the field

Place 2–3 pieces of corn in a vial and fill the vial halfway full with acetone, and allow to rest for 5 to 10 minutes, swirling occasionally. With a pipette, remove half of the solvent to a *clean, dry vial* and evaporate to dryness on a hotplate. Fill

this vial halfway full with Au NPs and add 2 drops of NaCl solution, then cap and shake the vial gently to mix. Insert into the vial attachment on Misa for measurement.

Table 2. Requirements for field test protocol

ID Kit - Au NP	6.07506.440
includes:	Gold nanoparticles (Au NP)
	Scoop
	Disposable pipettes
	2 mL glass vials
Reagents	
Acetone	
NaCl solution	3 g NaCl in 100 mL water
Test settings	Use ID Kit OP on MISA

CONCLUSION

Misa offers a facile, green, and economical method for sensitive detection of malathion sprayed on corn ears. Based on the unoptimized protocol reported in this application note, Misa

provides sufficient sensitivity for detecting malathion at concentrations that approximate or exceed the US maximum residue limit for sweet corn.

CONTACT

メトロームジャパン株式会社
143-0006 東京都大田区平
和島6-1-1
null 東京流通センター アネ
ックス9階

metrohm.jp@metrohm.jp

CONFIGURATION



MISA Advanced

Metrohm Instant SERS Analyzer (MISA) は、微量レベルでの違法物質、食品添加物、および食品汚染物質の迅速な検出 / 同定のための高性能な携帯可能分析システムです。MISAは、Metrohm 独自の軌道ラスタスキャン技術 (Orbital Raster Scan Technologie, ORS) を備えた高効率の分光器を有しています。これは省スペースで、より長いバッテリー寿命を持ち、現場やラボでの移動式用途にも完璧に適しています。MISA ではフレキシブルなサンプル採取を可能にする、レーザークラス1の様々なアタッチメントをご利用いただけます。アナライザーはBluetoothまたはUSBコネクタを介して操作可能です。

MISA Advanced パッケージは、ユーザーに Metrohmのナノ粒子溶液とP-SERSストリップを用いたSERS分析を可能にするコンプリートパッケージです。

MISA Advanced パッケージには、MISAバイアルアタッチメント、P-SERSアタッチメント、ASTM校正標準、USBミニケーブル、USB電源装置、ならびにMISA装置を操作するためのMISA Calソフトウェアが含まれます。装置と付属品を安全に保管するための頑丈な保護ケースも同梱されています。



ID - Au NP

IDキット - Au NPには、Mira/Misaユーザーが金コロイド溶液でSERS分析を行うのに必要なコンポーネントが含まれています。このキットには、使い捨てのへら、滴下ピペット、サンプルボトル、および金コロイド入りのボトルが含まれています。