

Identification of Forensic Fabrics Using a Portable Raman Spectrometer

At a crime scene, a police officer collects a fiber sample that may prove to be invaluable evidence in identifying a criminal or exonerating an innocent person. While FTIR has been used for analysis in the past, the strong absorption of the fabric or the glass slide where it is mounted makes the spectrum very hard to interpret. In recent years, Raman spectroscopy has been

studied extensively for forensic fiber analysis because of the high selectivity of Raman signatures, non-destruction nature of the test, and the ability to conduct the analysis without any sample preparation. The Raman test can be performed directly on fabrics or fibers mounted on glass slide with very little interference from the mounting resin or the glass.

EXPERIMENTAL

In this study, six types of undyed fabric samples were tested: diacetate, bleached cotton, polyester, polyamide (nylon), acrylic, and wool. A B&W Tek i-Raman EX portable Raman spectrometer with 1064 nm laser excitation along with a fiber optic probe holder was used. The video microscope sampling accessory can be used for testing on thin fibers and is very useful for microsamples, and for looking at specific spots on a sample.

The identification test involves creating a library and comparing each individual fabric spectrum with the spectra in the library. The software BWID was used to generate the library as well as to conduct the identification. The resulting "Match" or "No Match" is based on HQI (hit quality index), which measures the level of correlation of the sample spectrum against a reference spectrum calculated by using the correlation coefficient algorithm. The HQI threshold for a "Match" result was set at 80, which indicates an 80% correlation score between the sample spectrum and the reference spectrum.

Four out of the six types of fabrics are unambiguously identified. The overlaid spectra for these four fabrics are shown in **Figure 1**. As demonstrated in the diagonal line in the comparison results of **Table 1**, there is clear differentiation to separate diacetate, bleached cotton, polyamide, and acrylic fabrics.



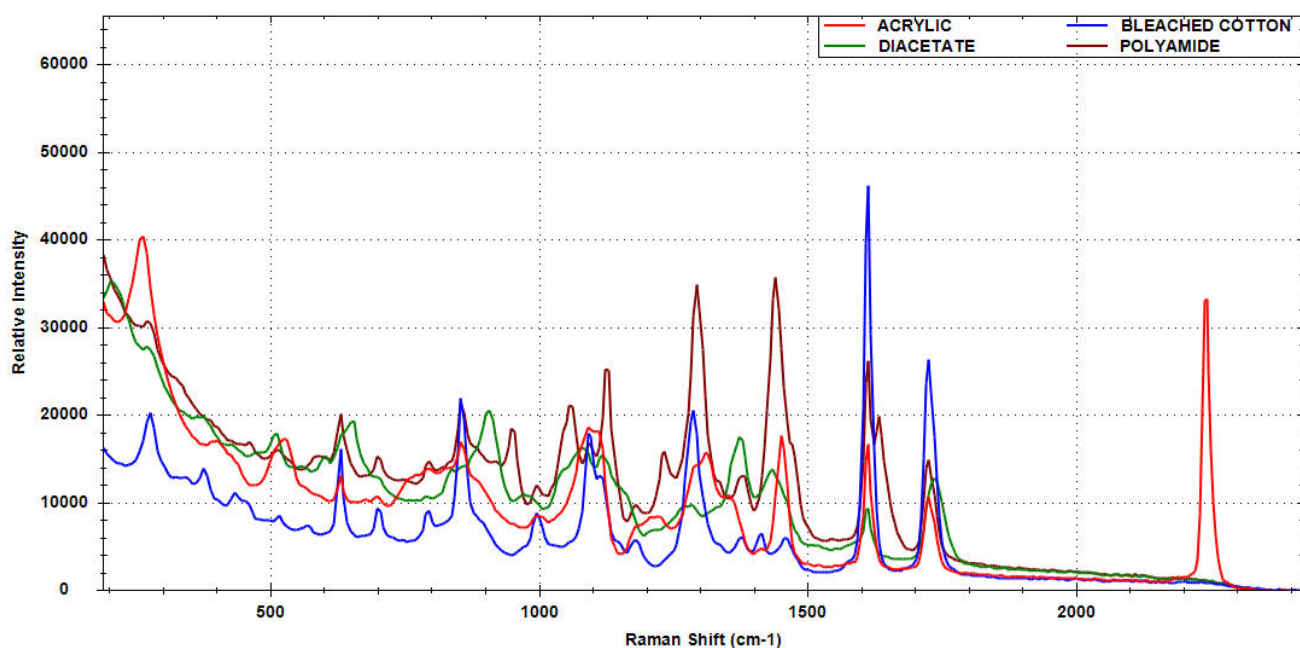


Figure 1. Overlay of spectra for acrylic, bleached cotton, polyamide, and diacetate

Library Sample	Diacetate	Bleached Cotton	Polyamide	Acrylic	Polyester	Wool
Diacetate	Match (HQI=87.68)	No match	No match	No match	No match	No match
Bleached Cotton	No match	Match (HQI=94.08)	No match	No match	No match	No match
Polyamide	No match	No match	Match (HQI=91.98)	No match	No match	No match
Acrylic	No match	No match	No match	Match (HQI=93.97)	No match	No match
Polyester	No match	No match	No match	No match	Match (HQI=96.59)	2 nd Match (HQI=81.23)
Wool	No match	No match	No match	No match	2 nd Match (HQI=94.75)	Match (HQI=85.38)

Table 1. Identification results using BWID software

Polyester and wool are difficult to differentiate by HQL, as the Raman spectra are highly similar (Figure 2). However, since fibers made from animal hair contain protein keratin, an amide I band from the amino acid cysteine in the region from 1600-1690 cm^{-1} would be expected[1] for wool and not polyester. In addition, since cysteine provides the disulphide crosslinks that

hold the polymer chains in wool, a disulphide S-S band at 523 cm^{-1} would also be expected[1]. These two peaks that are distinctively related to animal proteins can be seen in the wool spectrum shown in Figure 2, with the amide I band at 1653 cm^{-1} and the S-S band at 523 cm^{-1} . These two unique peaks can be used to differentiate wool from polyester.

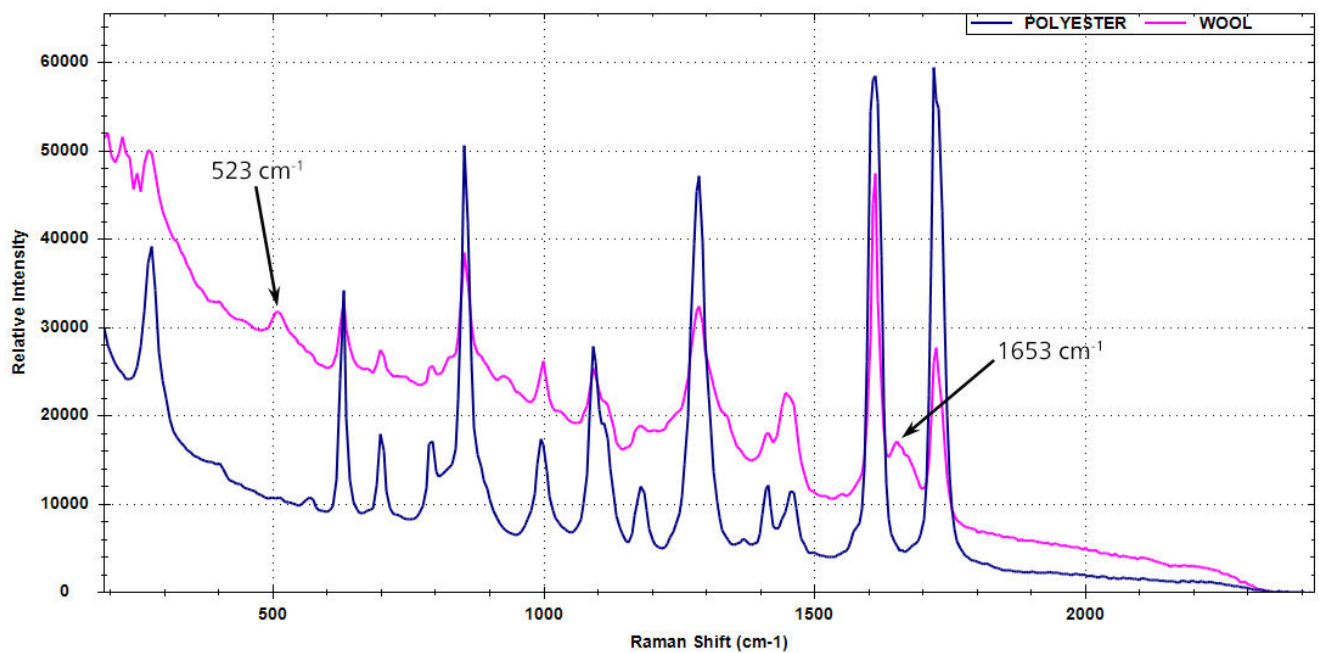


Figure 2. Overlay of spectra for wool and polyester

CONCLUSION

With unique discrimination power, Raman spectroscopy is a powerful technology that can be applied to forensic fabric and fiber analysis. Identification of an unknown fabric is achieved

in several minutes, making it a practical choice for rapid identification either on site or in the forensic lab.

REFERENCE

1. Li-Ling Cho. Identification of textile fiber by Raman microspectroscopy. J Forensic Science 2007; 6 (1):55-62

CONTACT

メトロームジャパン株式会社
143-0006 東京都大田区平
和島6-1-1
null 東京流通センター アネ
ックス9階

metrohm.jp@metrohm.jp

CONFIGURATION



BWID ID

ユーザーが作成したライブラリ、著作権で保護された B&W Tek のライブラリ、ならびに第三者プロバイダのライブラリに基づく材料の迅速な識別または検証を可能にする、B&W Tek 社製 携帯型ラマン spektrometer のためのデータ記録、材料識別、およびレポート作成のためのソフトウェア。システムの性能検査を含みます。ユーザーライセンスを包括。購入日より1年間の無料アップグレードを含みます。

(1064 nm)

ラボおよび産業用のB&W Tek社製ラマンプローブを用いた使用のためのビデオマイクロスコープ付きサンプル採取システム。作動距離16 mmで20倍拡大の対物レンズ付き。X、Y、およびZ軸方向の粗調整ならびに微調整、ターゲティング用同軸LED照明、サンプル観察のためのビデオカメラが使用可能であり、標準マイクロスコープ対物レンズと互換性があります。プローブは含まれておらず、個別にご購入いただけます。1064 nmコンフィグレーション。

BAC151C-1064

