


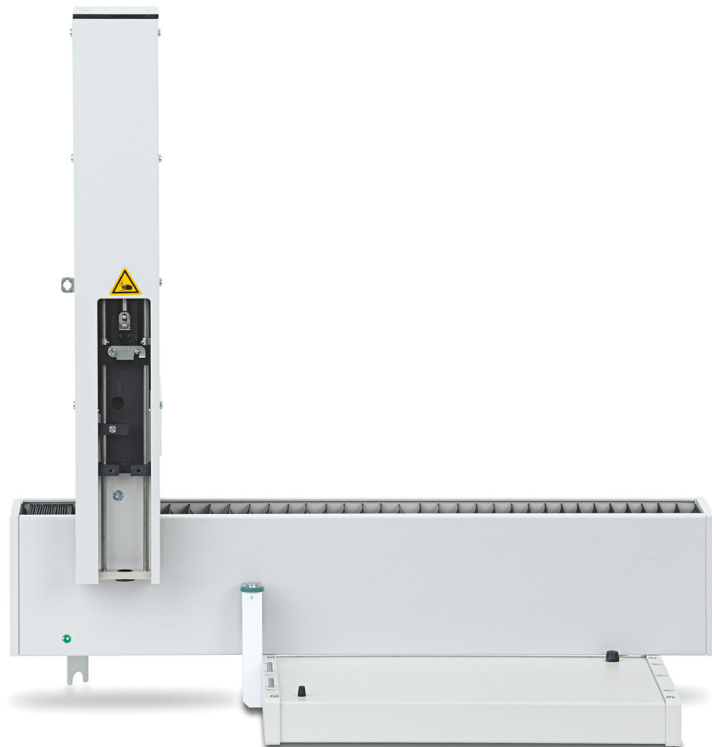

MMS 5000 Autosampler (AJ)

2.136.0800

Autosampler MMS 5000 (AJ) made by Analytik Jena for use with the Metrohm Combustion IC for fully automatic analysis of liquid and solid samples. To adapt the modular Multi-Matrix sampler to the correct sample type, either the liquids kit (6.7303.000) of the solids kit (6.7302.000) must be used.

Below, the accessories are grouped into Scope of delivery and Optional accessories.
Please keep this printout at hand for ordering replacement material.
These lists may be subject to change.


Scope of delivery 2.136.0800

Qt.	Order no.	Description
-----	-----------	-------------

MMS 5000 Autosampler (AJ) from Analytik Jena for use with the Metrohm Combustion IC for fully automatic analysis of liquid and solid samples. In order to match the modular Multi-Matrix sampler with the correct sample type, either the liquid kit (6.7303.000) or the solid kit (6.7302.000) must be used.




Optional accessories

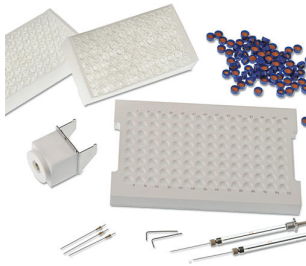Order no.	Description
6.7302.000	Kit for solid samples for MMS 5000, 35 positions Kit for solid samples for MMS 5000 with rack for sample boats, grippers and 10 quartz glass boats. 
6.7302.100	Quartz boat 40 x 9 mm (AJ) Quartz glass boat for sample injection in Combustion Module, 10 pcs. 
6.7303.000	Kit for liquid samples for MMS 5000, 112 positions Kit for liquid samples for MMS 5000 with rack for sample vessels, 100 µL syringe with replaceable needle and 100 snap-ring bottles. 
6.7303.100	Glass vial, 1.5 mL, 100 pieces For use with the following sample changers: Liquid Autosampler CIC (TEI), MMS 5000 Autosampler (AJ) and 889 Sample Center. 

6.7303.110 Septum for 67303100, 100 pieces

For use with the 67303100 Glass vial on the following sample changers:
Liquid Autosampler CIC (TEI), MMS 5000 Autosampler (AJ), and 889
Sample Center.



6.7303.200 50 μ L syringe with replaceable needle

Replacement syringe for MMS 5000 liquid setup




6.7303.210 100 μ L syringe with replaceable needle

Replacement syringe for MMS 5000 liquid setup



6.7303.220 Needles for 50 μ L/100 μ L syringes, 3 pcs.

Replacement needle for syringe for MMS 5000 liquid setup



6.7301.150

Substrate made of quartz for liquid samples

Substrate for liquid sample injections, 3 pcs.



6.7302.310

Sample rack 35 positions for solid samples

For solids.



6.7303.310

Sample rack 112 positions for liquid samples

For liquid samples.

