



898 XYZ Sample Changer 48 x 250 mL

2.898.0210

The 898 XYZ Sample Changer convinces with its speed and the number of samples that can be processed without supervision. Two sample racks with 24 x 250 mL beakers each can be fitted on the Sample Changer and processed continuously there. As soon as the processing of the first sample rack has been completed, it can be replaced with a rack with new samples. The sensors used are always in top condition, thanks to the built-in washing station with membrane pump. The control takes place via computer operation using the tiamo™ titration software.

Below, the accessories are grouped into Scope of delivery and Optional accessories. Please keep this printout at hand for ordering replacement material. These lists may be subject to change.

Scope of delivery 2.898.0210

Qt.	Order no.	Description
-----	-----------	-------------



Eluent canister for Online-IC instruments.



Sleeve with SGJ 14/12 mm and O-ring.



Sample beaker, clear glass, 250 mL, suitable for sample racks:
6.2041.310, 6.2041.400, 6.2041.430, 6.2041.510, 6.2041.820,
6.2068.020 and 6.2068.030, 1 piece



5 PCS

6.1446.000

SGJ stopper / B-14/(15)



3 PCS

6.1446.010

Stopper

Used with Sample Changers



1 PCS

6.1458.010

Titration head, 6 x SGJ 14 and 3 x SGJ 9 openings.

With 6xSGJ 14 and 3x SGJ 9 openings.



2 PCS

6.1543.200

Titration tip / M6 thread

Titration tip with antidiffusion valve.



2 PCS

6.1621.110

Cap for 30-L canister

Cap for 30-L canister. For easy and secure transportation of filled canisters.



2 PCS

6.1805.530

FEP tubing / M6 / 2 m

With light and kink protection



3 PCS

6.2709.070

Guiding sleeve

For fixation of buret and dosing tips in titration heads and electrode holders



1 PCS

6.6067.000

USB Stick for 898 XYZ Sample Changer




1 PCS

6.2071.040

Sample rack for 898 XYZ SC 24 x 250 mL left

Sample rack for 24 x 250 mL beakers (6.1432.320) for the 898 XYZ Sample Changer. The sample rack has a recess for the external rinsing station and is numbered from 1 - 24. It is positioned on the left half of the sample changer. There is sufficient space for a maximum of two sample racks per 898 XYZ SC.

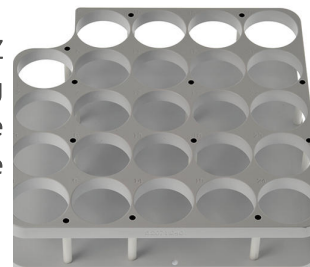


1 PCS



6.2071.050

Sample rack for 898 XYZ SC 24 x 250 mL right

Sample rack for 24 x 250 mL beakers (6.1432.320) for the 898 XYZ Sample Changer. The sample rack has a recess for the external rinsing station and is numbered from 25 - 48. It is positioned on the right half of the sample changer. There is sufficient space for a maximum of two sample racks per 898 XYZ SC.

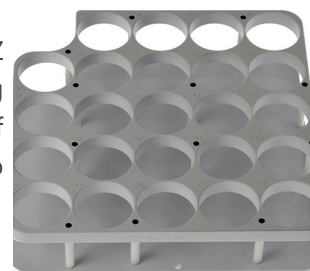

Optional accessories

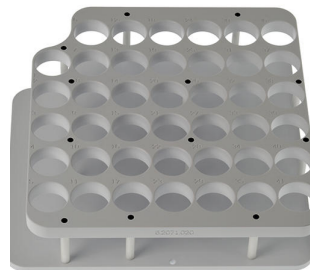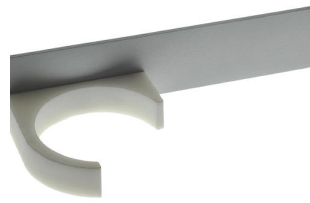Order no.	Description	
6.2071.020	Sample rack for 898 XYZ SC 41 x 120 mL left	
	Sample rack for 41 x 120 mL beakers (6.1459.300) for the 898 XYZ Sample Changer. The sample rack has a recess for the external rinsing station and is numbered from 1 - 41. It is positioned on the left half of the sample changer. There is sufficient space for a maximum of two sample racks per 898 XYZ SC.	
6.2071.030	Sample rack for 898 XYZ SC 41 x 120 mL right	
	Sample rack for 41 x 120 mL beakers (6.1459.300) for the 898 XYZ Sample Changer. The sample rack has a recess for the external rinsing station and is numbered from 42 - 82. It is positioned on the right half of the sample changer. There is sufficient space for a maximum of two sample racks per 898 XYZ SC.	
6.7600.010	898 XYZ Sample Changer drip pan	
	Drip pan for 898 XYZ Sample Changer.	
6.7600.020	898 XYZ Sample Changer rinsing station holder	
	Rinsing station holder for 898 XYZ Sample Changer.	

6.7600.030 898 XYZ Sample Changer rinsing station

Rinsing station for 898 XYZ Sample Changer.



6.7600.040 898 XYZ Sample Changer tubing guide

898 XYZ Sample Changer tubing guide



6.7600.050 898 XYZ Sampler Changer titration head holder

898 XYZ Sampler Changer titration head holder



6.7600.060 898 XYZ Sample Changer safety shield

898 XYZ Sample Changer safety shield



6.7600.070

898 XYZ Sample Changer rinse and extraction kit


898 XYZ Sample Changer rinse and extraction kit (FEP/TYGON).



6.7600.080

898 XYZ Sample Changer rinse reduction kit

898 XYZ Sample Changer rinse reduction kit.

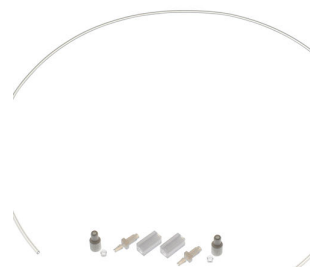

6.7600.090

898 XYZ Sample Changer 24 volt power supply unit

898 XYZ Sample Changer 24 volt power supply unit.

