


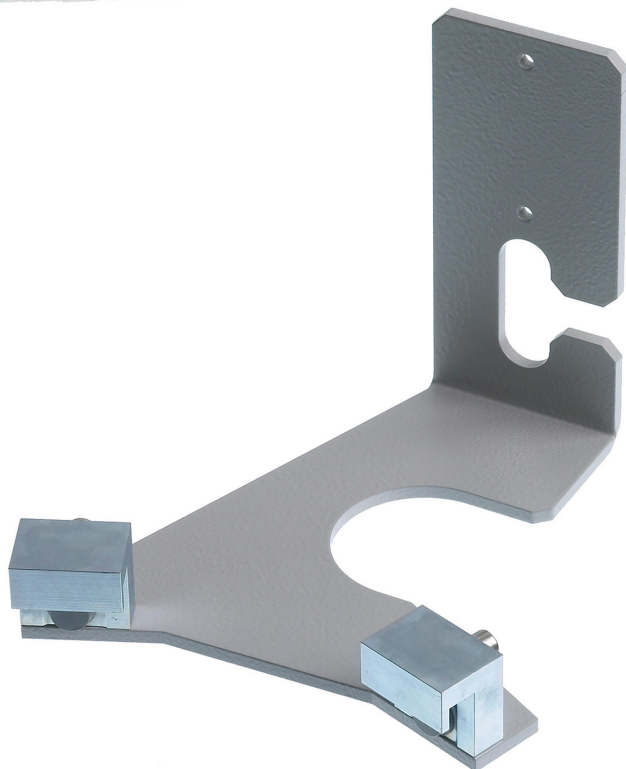

# Support pour tige d'ionisation pour 864 Robotic Balance Sample Processor

6.2057.160

## Accessoires optionnels

| Order no.  | Description                                                                                                                               |
|------------|-------------------------------------------------------------------------------------------------------------------------------------------|
| 6.9013.000 | Ionisation rod for ionizer<br><br>The ionisation rod is mounted with the holder (6.2057.160) to the 864 Robotic Balance Sample Processor. |

