


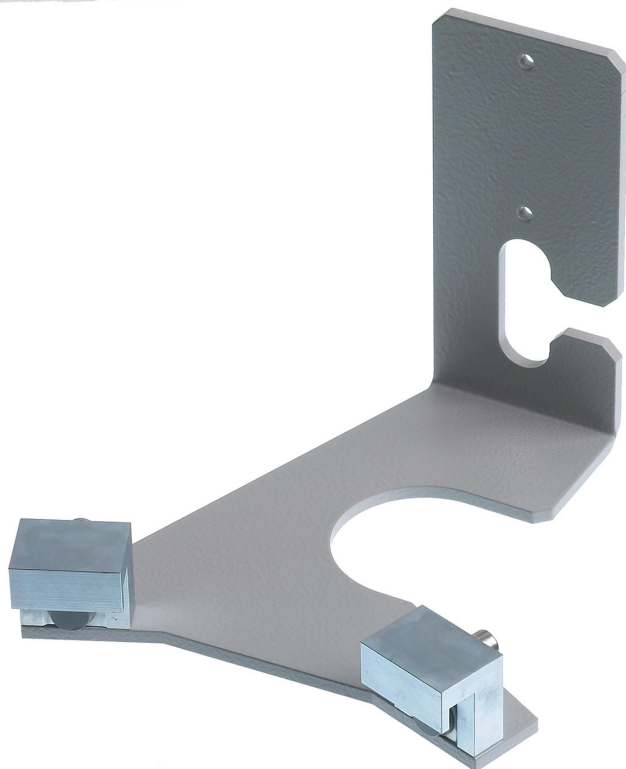

Holder for ionization rod for 864 Robotic Balance Sample Processor

6.2057.160

オプションアクセサリ

Order no.	説明
6.9013.000	Ionisation rod for ionizer

