


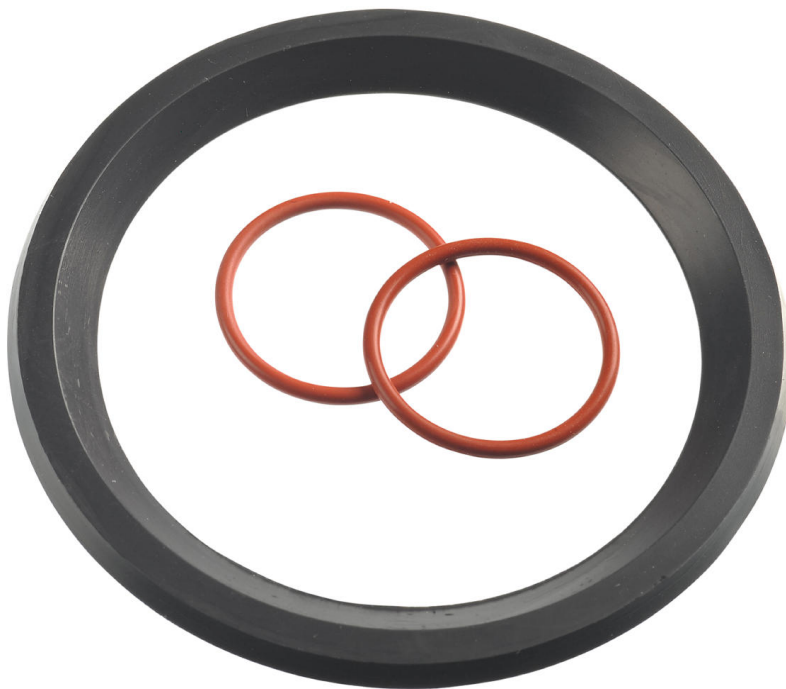

Set of seals for Karl Fischer titration cell

6.01408.010

Complete set of seals, suitable for 6.05609.000 and 6.05609.010.

Phạm vi giao hàng 6.01408.010

Qt.	Order no.	Description
1 PCS	6.1454.130	Form seal made of FPM for 61414xxx for KF and VA instruments

