


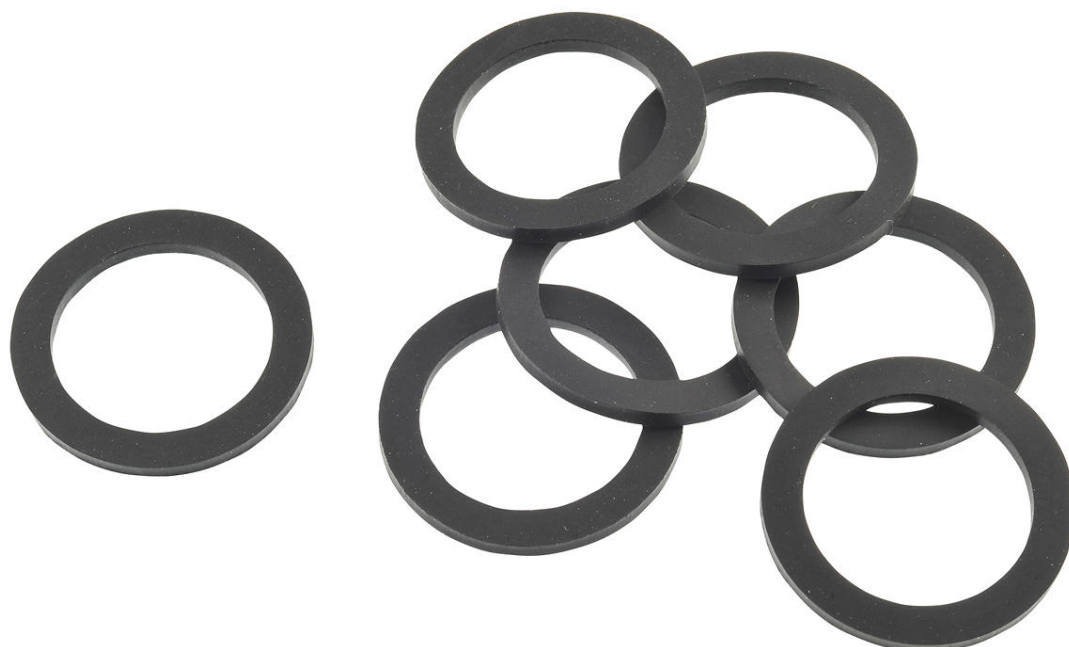

Consumable Kit seals for the 6.02710.010 KF Dis-Cover lid

6.05700.170

Replacement seals for 6.02710.010 lid, 16 pieces

Phụ kiện tùy chọn

Order no.	Description
6.02710.010	KF Dis-Cover lid for OMNIS 120 mL sample beaker, 16 pieces

Lid with seals for volumetric Karl Fischer Titration in 6.01400.200, 6.01400.300 and 6.01400.303 sample beakers in the OMNIS Sample Robot Pick&Place system.

