


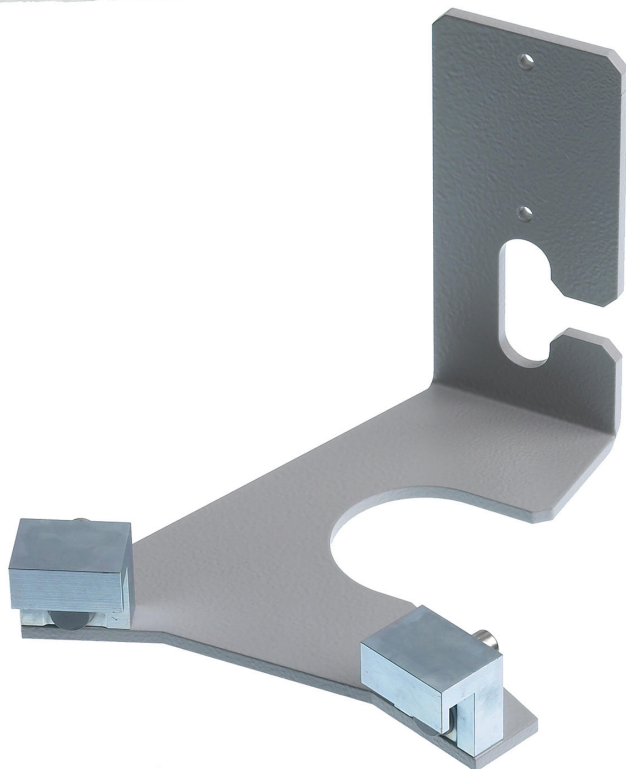

Holder for ionization rod for 864 Robotic Balance Sample Processor

6.2057.160

Phụ kiện tùy chọn

Order no.	Description
6.9013.000	Ionisation rod for ionizer The ionisation rod is mounted with the holder (6.2057.160) to the 864 Robotic Balance Sample Processor.

