


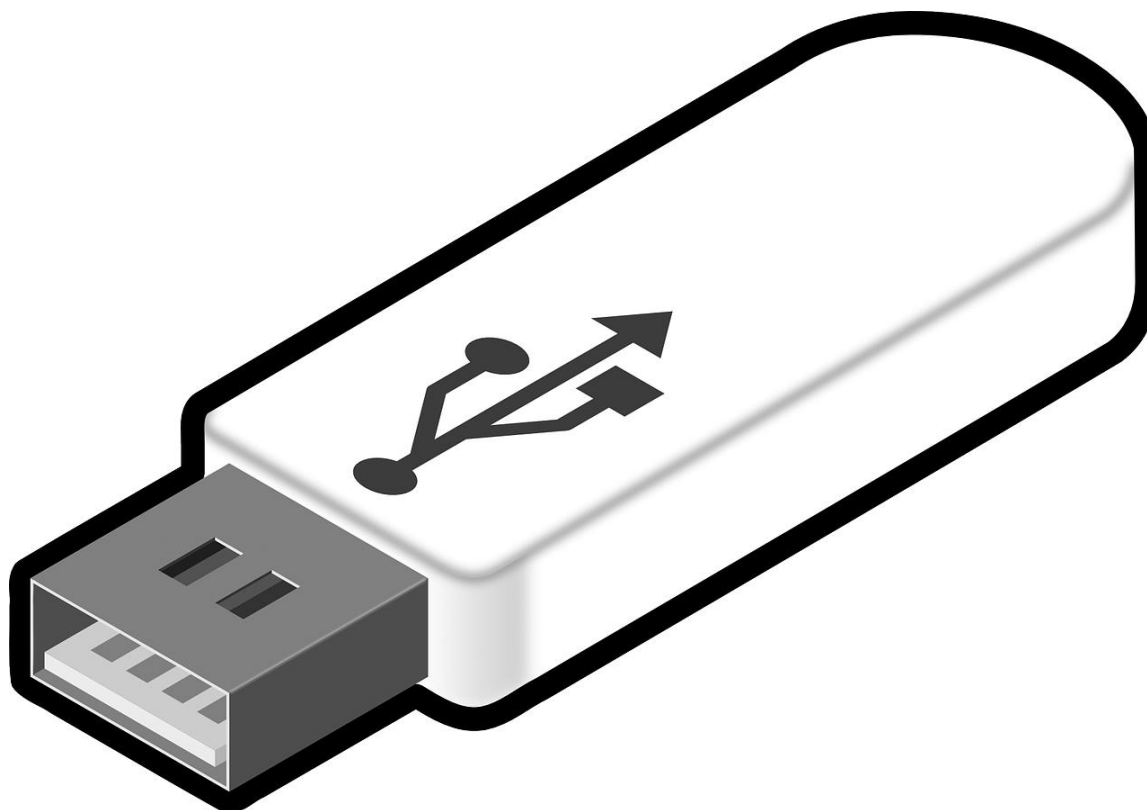

Metrohm IC Driver 1.0, ICP-MS MassHunter

6.6090.100

Software drivers for integrating Metrohm IC instruments in Agilent's ICP-MS MassHunter Software 5.3 and higher.

Learn more about the coupling of IC and mass spectrometers

Phụ kiện tùy chọn

Order no.	Description
6.2148.010	Remote Box MSB Additional remote interface for the connection of devices that can be controlled via remote lines. With permanently attached cable.



6.05330.400 IC equipment, connection Agilent ICP-MS

IC equipment for the connection and bidirectional control of Metrohm IC and Agilent ICP-MS (IC-ICP/MS)

