


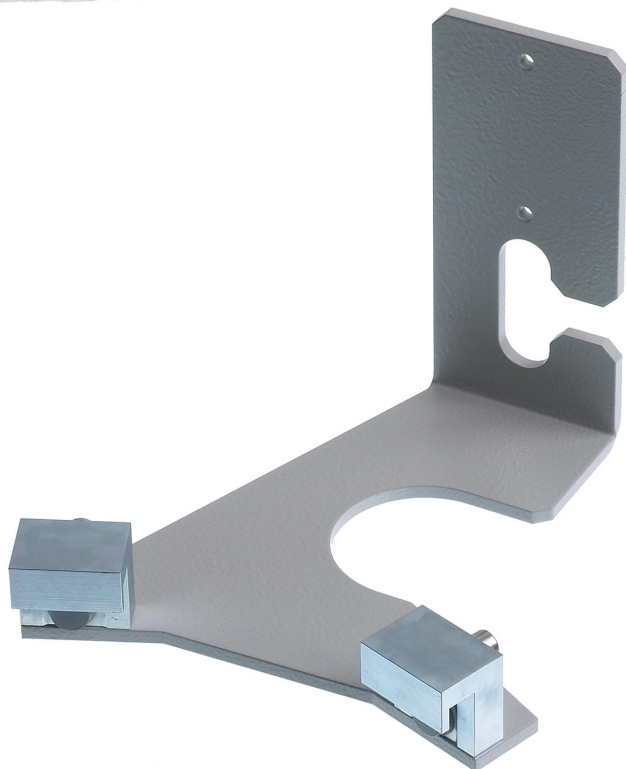

# 用于 864 Robotic Balance Sample Processor 的电离棒的支架

6.2057.160

## Optional accessories

| Order no.  | Description                                                                                                                               |
|------------|-------------------------------------------------------------------------------------------------------------------------------------------|
| 6.9013.000 | Ionisation rod for ionizer<br><br>The ionisation rod is mounted with the holder (6.2057.160) to the 864 Robotic Balance Sample Processor. |

