



Application Note AN-C-185

根据美国药典(USP)测定碳酸氢钾和氯化钾泡腾片口服混悬液中的钾

Method validation according to the U.S. Pharmacopoeia

Potassium bicarbonate and potassium chloride effervescent tablets for oral solution are used to prevent hypokalemia (low levels of potassium in blood) [1]. Pharmaceutical manufacturers and laboratories must use approved quality monitoring techniques for drugs and formulations as stipulated by U.S. Pharmacopoeia (USP) monographs.

As an alternative to flame photometry, ion chromatography with non-suppressed conductivity detection has been approved by the USP as a validated method to quantify

potassium content in potassium bicarbonate and potassium chloride effervescent tablets for oral solution [2].

The Metrosep C 6 - 150/4.0 column ([L76](#)) provides the required separation of potassium and magnesium. All acceptance criteria from the USP monograph «Potassium Bicarbonate and Potassium Chloride Effervescent Tablets for Oral Solution» are fulfilled [2]. The present IC method has been validated according to USP General Chapter <621> Chromatography, system suitability [3].

SAMPLE AND SAMPLE PREPARATION

Sample solutions are prepared from commercially available potassium bicarbonate and potassium chloride effervescent tablets for

oral solution. Standard analyses are performed with a solution of USP Potassium Chloride RS. No additional sample preparation is required.

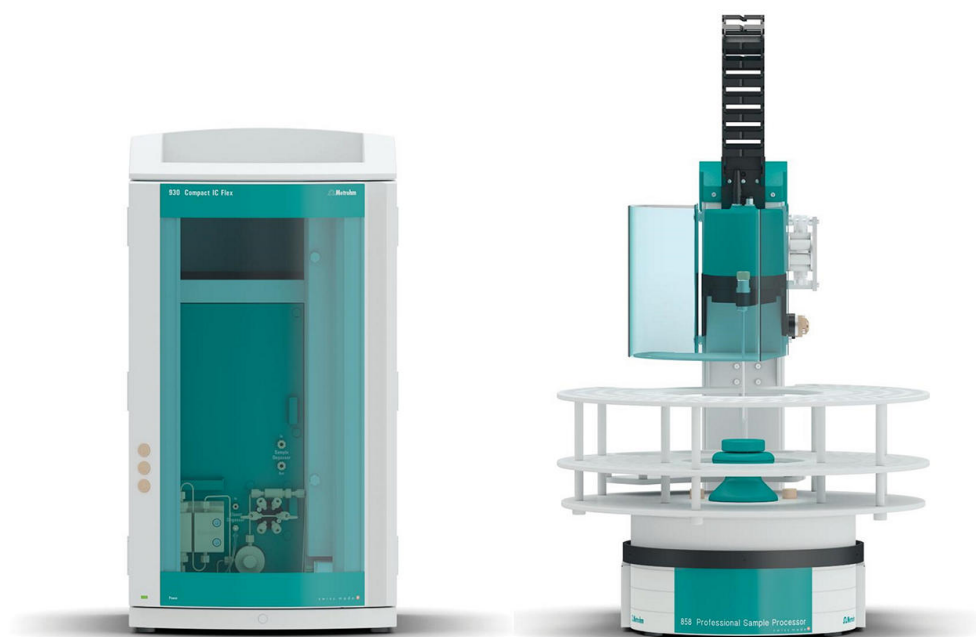


Figure 1. Instrumental setup including a 930 Compact IC Flex Oven and an 858 Professional Sample Processor.

EXPERIMENTAL

The sample stock solution is prepared through the addition of 25 g finely powdered potassium bicarbonate and potassium chloride effervescent tablets for oral solution to a 1000 mL volumetric flask. The powder is dissolved in 200 mL ultrapure water. After effervescence ceases, the volumetric flask is filled up to the mark. This stock solution contains nominally 4809.48 mg/L potassium. A 1.533 mL aliquot of this stock solution is transferred to a 500 mL volumetric flask and is filled up to the mark with ultrapure water. This final sample solution nominally contains 15.0 µg/mL potassium.

A working standard solution of 15 µg/mL potassium chloride is prepared from the respective USP reference standards.

All solutions (i.e., samples and standards) are injected directly into the ion chromatograph (**Figure 1**) using an 858 Professional Sample Processor. Potassium is separated from all other cations using the Metrosep C 6 - 150/4.0 column (L76).

The calibration is performed by using a 6-point linear calibration curve in the concentration range of 3.75–22.5 µg/mL potassium. The sample is then analyzed in duplicate.

Table 1. Requirements for the IC method as per USP Monograph «Potassium Bicarbonate and Potassium Chloride Effervescent Tablets for Oral Solution» [2].

Column with L76 packing	Metrosep C 6 - 150/4.0
Eluent	4 mmol/L nitric acid
Flow rate	0.9 mL/min
Temperature	30 ° C
Injection volume	20 µL
Detection	Direct conductivity

RESULTS

The IC assay for potassium content was validated according to USP Monograph «Potassium Bicarbonate and Potassium Chloride Effervescent Tablets for Oral Solution» [2]. The accuracy of the potassium determination was calculated as 105% (Table 2 and Figure 2).

All acceptance criteria were fulfilled, e.g., the correlation coefficient for potassium was 0.9999, the resolution of adjacent peaks, and the relative standard deviation of the standard solutions was <0.15% (n = 6) (Table 2).

Table 2. Required acceptance criteria according to USP Monograph Potassium Bicarbonate and Potassium Chloride Effervescent Tablets for Oral Solution [2] (Abbreviations: K⁺, potassium; Mg²⁺, magnesium).

Parameter	Actual	USP requirement	Status
% RSD	0.15	NMT 1.0	Pass
Tailing factor	1.37	NMT 2.0	Pass
Recovery	104.8%	90–110%	Pass
Resolution K ⁺ /Mg ²⁺	4.17	NLT 2.0	Pass

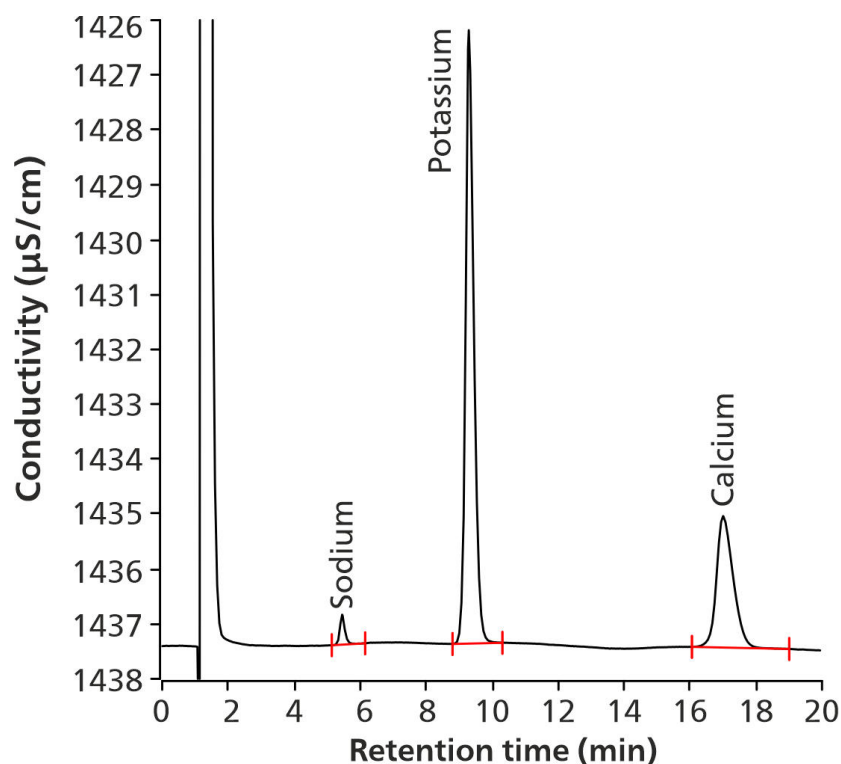


Figure 2. Chromatogram of the sample solution (105% recovery of the nominal concentration for potassium). Sodium and calcium were not quantified. The resolution was 11, for both pairs sodium/potassium and potassium/calcium.

CONCLUSION

The presented IC method for the determination of potassium content in potassium bicarbonate and potassium chloride effervescent tablets for oral solution using the Metrosep C 6 column (packing material L76) for separation is officially included into the USP [2]. Robustness and reliability of the method was demonstrated

following the guidelines of the USP General Chapter <621> [3]. The presented setup is suitable to quantify potassium according to the USP requirements. Additional USP methods are summarized in the flyer «[Bring your USP methods up to date!](#)» [4].

REFERENCES

1. Kardalas, E.; Paschou, S. A.; Anagnostis, P.; et al. Hypokalemia: A Clinical Update. *Endocr Connect* **2018**, 7 (4), R135–R146. <https://doi.org/10.1530/EC-18-0109>.
2. *Potassium Bicarbonate and Potassium Chloride Effervescent Tablets for Oral Solution*; Monograph; U.S. Pharmacopeia/National Formulary: Rockville, MD. https://doi.org/10.31003/USPNF_M67253_02_01.
3. <621> *Chromatography, General Chapter*, U.S. Pharmacopeia/National Formulary: Rockville, MD. <https://www.uspnf.com/notices-gc-621-nitr-20220826>.
4. Metrohm AG. Bring Your USP Methods up to Date!, 2023. [8.000.5436EN](https://www.metrohm.com/asset/documents/8.000.5436EN)

Internal reference: AW IC IN6-1887-052018

CONTACT

瑞士万通中国
北京市海淀区上地东路1号
院1号楼7层702
100085 北京

marketing@metrohm.com.cn

CONFIGURATION



Metrosep C 6 - 150/4.0

高容量的 C 6 材料使分离柱 Metrosep C 6 - 150/4.0 成为在浓度差异很高时的正常保留时间内分离标准阳离子的解决方法。可用此柱测定铵含量很高的饮用水。



Metrosep C 6 Guard/4.0

Metrosep C 6 Guard/4.0 包含 C-6 柱材料,用于防微粒和防污染。用它可显著延长分析用分离柱的使用寿命。Metrosep C 6 Guard/4.0 按照 «On Column Guard System» 来运行,可几乎无死点容积地直接安装到相应分离柱上。



930 Compact IC Flex Deg

930 Compact IC Flex Deg 是智能型的**无抑制** Compact IC 仪器,且内置**脱气装置**。该仪器可使用各种分离和检测方法。

典型的应用范围:

- 阴离子或阳离子测定,无抑制的电导检测
- 使用 UV-VIS 或安培检测的简单应用



858 Professional Sample Processor

858 Professional Sample Processor 可处理体积在 500 µL 至 500 mL 之间的样品。进行样品转移时,既可以使用 850 Professional IC System 上的蠕动泵、也可通过 800 Dosino 来进行。