



Application Note AN-S-375

Fluoride in sodium fluoride for pharmaceutical use

Method validation according to the U.S. Pharmacopeia

Dental care products like toothpaste often contain sodium fluoride to support tooth enamel remineralization and prevent dental cavities (caries) [1]. The WHO recommends 1000–1500 mg/L fluoride in toothpaste for adults to prevent tooth decay [2]. Manufacturers use the United States Pharmacopeia and National Formulary (USP-NF) Monograph «Sodium Fluoride» to quantify sodium fluoride and its anionic contaminants chloride and acetate in dental care products [3].

The validated USP method proposes ion chromatography (IC) with suppressed

conductivity detection to carry out the fluoride assay as well as the impurity determination in a single chromatogram [3]. The demonstrated IC method uses the Metrosep A Supp 16 - 250/4.0 (L91) column and a hydroxide eluent, complying with all parameters given in the USP Monograph «Sodium Fluoride» [3]. It provides excellent separation of fluoride, acetate, and chloride, and fulfills all acceptance criteria of the Monograph. The IC method has been validated according to USP General Chapters <621> Chromatography [4] and <1225> Validation of Compendial Procedures [5].

STANDARD AND SAMPLE PREPARATION

The standard solutions and the system suitability solutions are prepared from the respective 1000 µg/mL certified standards by dilution with ultrapure water (UPW).

For the fluoride assay, the standard solution is obtained by diluting a sodium fluoride solution to 2 µg/mL. The system suitability solution contains 2 µg/mL sodium fluoride and 1 µg/mL sodium acetate. For the impurity test, the standard solution consists of 0.2 µg/mL sodium chloride in UPW. The system suitability solution for the impurity test contains 1 mg/mL sodium

fluoride and 1 µg/mL sodium chloride in UPW. Sample analyses are performed with a solution prepared from commercially available sodium fluoride salt. The sample solution is prepared by dissolving and diluting sodium fluoride salt with UPW to a nominal concentration of 2 µg/mL which corresponds to 0.9 µg/mL fluoride (for the assay). For the impurity test, samples were diluted to a nominal concentration of 1 µg/mL sodium fluoride.

No additional sample preparation is required.

EXPERIMENTAL

Samples and standard solutions were directly injected into the IC using a 919 IC Autosampler

plus (Figure 1).



Figure 1. Instrumental setup including a 930 Compact IC Flex, 919 IC Autosampler plus, and an 800 Dosino for automatic regeneration of the Metrohm Suppressor Module (MSM).

Fluoride was separated from acetate and chloride using a potassium hydroxide eluent and the column Metrosep A Supp 16 with column material L91 (**Table 1**). The analytes were quantified by evaluating their conductivity signal

after chemical suppression.

The calibration was performed using a single 2.0 µg/mL standard injected six times. The sample was analyzed in duplicate.

Table 1. Requirements for the IC method as per USP Monograph «Sodium Fluoride» [3].

Column with L91 packing	Metrosep A Supp 16 - 250/4.0
Eluent	15 mmol/L potassium hydroxide
Flow rate	1.0 mL/min
Temperature	40 ° C
Injection volume	20 µL
Detection	Conductivity with suppression

RESULTS

The IC assay for fluoride content was validated according to USP Monograph «Sodium Fluoride» [3]. Suitability requirements for resolution,

tailing factor, and relative standard deviation were fulfilled (**Table 2**).

Table 2. Suitability requirements for the assay.

Parameter (assay)	Actual	USP requirement	Status
Resolution F ⁻ /acetate	5.9	NLT 1.5	Pass
Tailing factor	1.1	NMT 2.0	Pass
RSD fluoride (%; n=5)	0.52	NMT 0.73	Pass

The chromatographic resolution between fluoride and acetate is shown in **Figure 2**. The recovery of fluoride for the sample analysis

(99.7%) was within the USP acceptance criteria (98–102%).

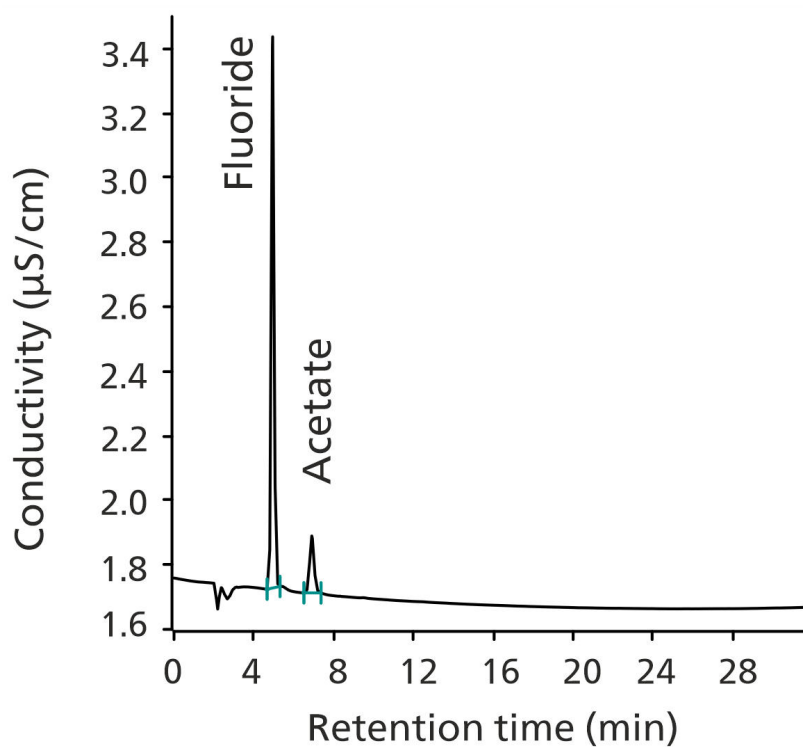


Figure 2. Chromatogram of the system suitability solution for the assay with 2.0 µg/mL sodium fluoride and 1.0 µg/mL sodium acetate.

Regarding the impurity tests for potential contamination with chloride, the IC method

showed excellent compliance with the USP requirements (**Table 3**).

Table 3. Suitability requirements for the impurities in sodium fluoride.

Parameter (impurity)	Actual	USP requirement	Status
Resolution F ⁻ /Cl ⁻	7.7	NLT 4	Pass
RSD fluoride (% , n=5)	4.2	NMT 5	Pass
S/N ratio Cl ⁻	>740	NLT 20	Pass

Figure 3 shows the chromatographic resolution

between fluoride and chloride.

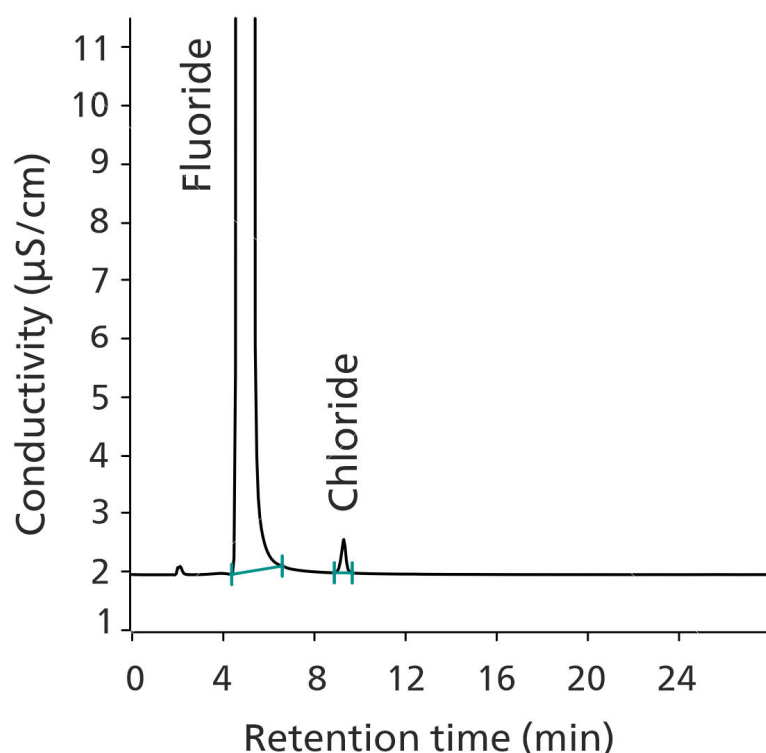


Figure 3. Chromatogram of the system suitability solution for the impurity chloride. The solution contained 1 mg/mL sodium fluoride and 1 μg/mL sodium chloride. The peaks are well resolved, and the signal-to-noise ratio for chloride was >740 (a value of more than 20 is required).

In all tested samples, the chloride content was (Table 4). well below the acceptance criteria of 0.012%

Table 4. Results of the chromatograms shown in Figures 2 and 3.

Anion	Sample ID	Result [%]	USP Limit [%]
1 Fluoride	Assay	99.7	98–102
2 Chloride	Impurity	0.0016	≤0.012

概要

The presented IC method is suitable to determine sodium fluoride and its impurities according to the USP Monograph «Sodium Fluoride». The method helps manufacturers of

dental care products to determine fluoride content as well as impurities more easily in toothpaste.

REFERENCES

1. Yeung, C. A. A Systematic Review of the Efficacy and Safety of Fluoridation. *Evid Based Dent* **2008**, 9 (2), 39–43.
<https://doi.org/10.1038/sj.ebd.6400578>.
2. WHO. A. 14 Fluoride Toothpaste – Dental Caries; Expert Committee on Selection and Use of Essential Medicines Application review; WHO, 2021.
3. Sodium Fluoride; Monograph; U.S. Pharmacopeia/National Formulary: Rockville, MD.
https://doi.org/10.31003/USPNF_M76470_04_01.
4. 〈621〉 Chromatography; General Chapter; U.S. Pharmacopeia/National Formulary: Rockville, MD.
https://doi.org/10.31003/USPNF_M99380_01_01.
5. 〈1225〉 Validation of Compendial Procedures; General Chapter; U.S. Pharmacopeia/National Formulary: Rockville, MD.
https://doi.org/10.31003/USPNF_M99945_04_01.

CONTACT

Metrohm Taiwan Ltd.
開封街二段 46 號 5 樓
108 台北市

info@metrohm.com.tw

CONFIGURATION




930 Compact IC Flex Oven/SeS/PP/Deg

930 Compact IC Flex Oven/SeS/PP/Deg 是智能型 Compact 离子色谱仪器,带有柱加热炉、序列抑制和蠕动泵用于抑制器再生,以及内置的脱气装置。该仪器可使用各种分离和检测方法。

典型的应用范围:

- 阴离子或阳离子测定,序列抑制法及电导检测

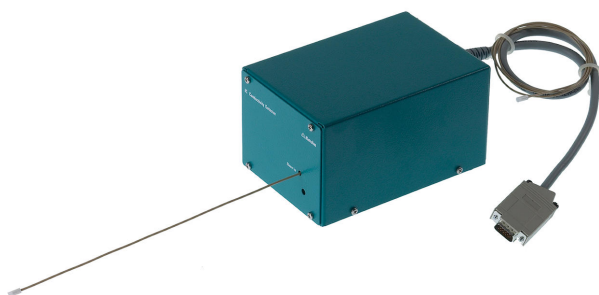

IC Conductivity Detector

用于智能型离子色谱仪的紧凑智能型高性能电导检测器。不凡的温度稳定性,受保护的检测器端子板内的整个信号处理过程以及新一代的 DSP(数字式信号处理)均能确保测量的准确性。归功于动态工作范围,无需进行范围变更(也不是自动进行)。



Metrosep A Supp 16 - 250/4.0

Metrosep A Supp 16 适用于大容量分离问题,即使在复杂的分离问题中也能保持优良的分辨率。Metrosep A Supp 16 分离柱基于表面作用的聚苯乙烯/二乙烯基苯共聚物。官能组均为共价键合。该特征以及表面结构使阴离子交换剂具有独特的选择性。大容量 Metrosep A Supp 16 适用于复杂的分离问题。

Metrosep A Supp 16 - 250/4.0 拥有优良的分辨率,可解决复杂的分离问题。该柱非常适用于监控电镀浴。可测定浓酸中的阴离子痕量。可在食品分析中用于测定麦芽糖衍生物,这只是大容量 Metrosep A Supp 16 - 250/4.0 的众多应用中的一种。



Metrosep A Supp 16 Guard/4.0

Metrosep A Supp 16 Guard/4.0 保护柱可有效保护分析用分离柱 Metrosep A Supp 16,使其免受污染。该保护柱采用 «On Column Guard System» 技术,其特征是操作简便。只要将其拧到分析柱上即可。不需要任何工具。



MSM A

抑制器转子,用于所有带MSM的IC仪器。



919 IC Autosampler plus

919 IC Autosampler plus 满足实验室内处理中等样品量的要求。使用该仪器,可实现万通产品的各种离子色谱分析自动化。