



Application Note AN-COR-012

ASTM G5:阳极电位极化测量

ASTM-compliant methods from Metrohm Autolab

The ASTM G5 is a standard method to test the corrosion of Type 430 stainless steel with a potentiodynamic anodic polarization measurement. The primary use of this test method is actually not in materials testing – it offers a simple way to confirm the accuracy of the test equipment (i.e., PGSTAT and corrosion

cell). With a Metrohm Autolab instrument and our ASTM-compliant corrosion cells, it is possible to meet the requirements of this ASTM standard. This Application Note describes an example measurement that was made using VIONIC powered by INTELLO according to the ASTM guidelines.

SAMPLE PREPARATION

It is critical that the sample surface is free from contamination. Directly before immersion in the corrosive medium, the sample (a 1 cm² disk of Type 430 stainless steel) was cleaned by a combination of mechanical polishing with

sandpaper and alternatively rinsing with ultrapure water and isopropyl alcohol. It is important that this is done just before immersing the sample in order to prevent the surface from recontamination.

EXPERIMENTAL

The sample was immersed in 1 N (0.5 mol/L) aqueous sulfuric acid and two Metrohm platinum sheet electrodes were used as the counter electrode. For the reference electrode, an Ag/AgCl 3 mol/L KCl Metrohm reference electrode was chosen. The cell used in this study was the ASTM-compliant 1 L Metrohm Autolab corrosion cell.

To minimize dissolved oxygen, the sulfuric acid solution was deaerated by bubbling nitrogen gas through it for one hour. The Type 430 stainless steel disk was immersed in the solution 30 minutes before the experiment during the N₂ bubbling step. A nitrogen blanket above the solution was maintained throughout the experiment in order to obstruct any atmospheric

oxygen diffusion into the solution.

A VIONIC potentiostat/galvanostat was used for the measurement. The procedure and data treatment were performed with the INTELLO software.

The ASTM G5 standard method requires that a voltage scan is initiated from the corrosion potential (E_{corr} , also known as the open-circuit potential OCP) to 1.60 V vs saturated calomel electrode (SCE) [1]. In this case, the reference electrode system employed was Ag/AgCl 3 mol/L KCl, so the end potential was adjusted to 1.630 V.

The data was plotted in accordance with the guidelines laid out with ASTM Standard Practice G3 [2].

RESULTS

The plot of current (I) vs potential (E) is shown in Figure 1.

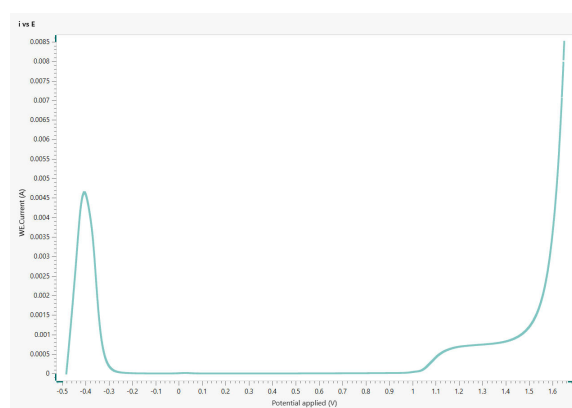


Figure 1. A plot of I vs E for the corroding sample of stainless steel in 0.5 mol/L sulfuric acid solution.

The data is transformed according to ASTM standard G3 in **Figure 2**, where a plot of the potential (E) vs the log of the current density (j) is shown.

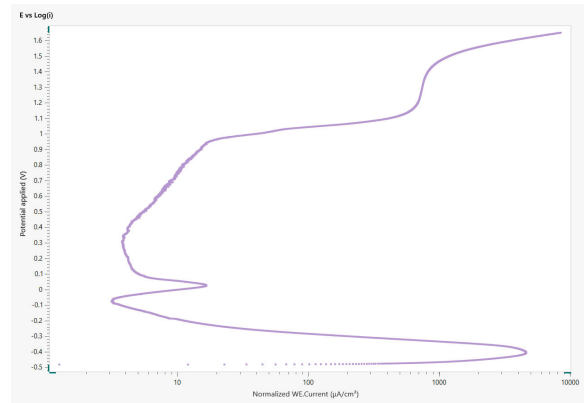


Figure 2. The corresponding plot of log(j) vs E for the corroding sample of stainless steel in 0.5 mol/L sulfuric acid solution.

The common features relating to the oxidation process of stainless steel in acidic solutions are more easily discernible in this plot. These features include the:

1. Active Region
2. Passive Region
3. Transpassive Region
4. Secondary Passivity Region

These four regions are highlighted in the plot in **Figure 3**.

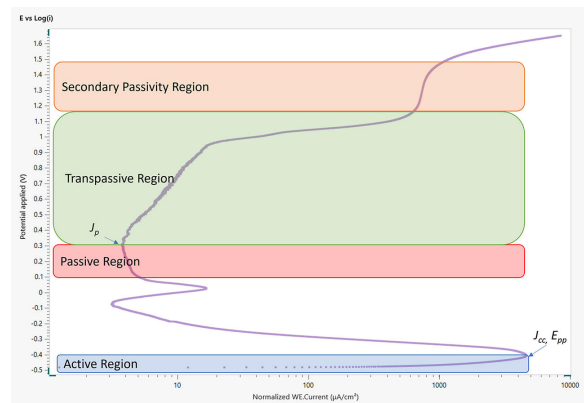


Figure 3. This plot is identical to Figure 2, but the regions in the plot are now highlighted. The Active Region is shown in blue, the Passive Region in red, the Transpassive Region in green, and the Secondary Passivity Region in orange.

The Active Region (**Figure 3**, in blue) is characterized by a large increase in the current density, corresponding to oxidation (corrosion) of the stainless-steel sample, until the primary passivation potential (E_{pp}) is reached. The E_{pp} also corresponds to a critical current density (j_{cc}). For potentials higher than the E_{pp} , the current density drops off, which is usually associated with the formation of a protective (passivating)

layer on the surface of the electrode.

After a small peak, the origin of which is likely related to active dissolution of stainless steel from a Cu-enriched layer [3], the current density does not change substantially from its passive current density value (j_p) even as the potential is increased. This is called the Passive Region (**Figure 3**, in red).

At potentials higher than where j_p occurs, the

current density increases again due to breaking the passive layer. This is termed the Transpassive Region (**Figure 3**, in green).

Beyond the Transpassive Region, the curve enters another section where the current density does not increase much with the applied

potential. This is termed the Secondary Passivity Region (**Figure 3**, in orange). Further from this, oxygen evolution can occur, which is not shown in **Figure 2**.

REFERENCES

1. *Standard Reference Test Method for Making Potentiodynamic Anodic Polarization Measurements.*
<https://www.astm.org/g0005-14r21.html>
(accessed 2024-03-08).
2. *Standard Practice for Conventions Applicable to Electrochemical Measurements in Corrosion Testing.*
<https://www.astm.org/g0003-14r19.html>
(accessed 2024-03-08).
3. Ruel, F.; Volovitch, P.; Peguet, L.; et al. On the Origin of the Second Anodic Peak During the Polarization of Stainless Steel in Sulfuric Acid. *Corrosion* **2013**, 69 (6), 536–542. DOI:10.5006/0820

CONTACT

Metrohm Taiwan Ltd.
開封街二段 46 號 5 樓
108 台北市

info@metrohm.com.tw

CONFIGURATION



VIONIC

VIONIC 是我们的新一代恒电位仪 / 恒电流仪, 由 Autolab 的新 INTELLO 软件提供动力。

相比目前市场上任何单一仪器, VIONIC 提供了全面的组合规格。

- 顺从电压: $\pm 50\text{ V}$
- 标准电流 $\pm 6\text{ A}$
- EIS 频率: 达 10 MHz
- 采样间隔: 低至 $1\mu\text{s}$

VIONIC 的价格中通常还包括大多数其他仪器产生的额外费用, 例如:

- 电化学阻抗谱 (EIS)
- 可选浮动配件
- 第二测量电极 (S2)
- 模拟扫描